

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027272.D
 Acq On : 10 Aug 2022 21:14
 Operator : SY/MD
 Sample : N4144-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027272.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	37	rVB	28049	31802	2.35%	0.313%
2	1.301	76	81	90	rBV	155846	158045	11.66%	1.555%
3	1.558	155	161	175	rVB	139817	164555	12.14%	1.619%
4	2.101	321	330	344	rBV	268946	375242	27.68%	3.691%
5	2.452	437	439	441	rBV2	793	531	0.04%	0.005%
6	2.895	575	577	579	rVB2	642	266	0.02%	0.003%
7	2.998	606	609	611	rBV2	699	356	0.03%	0.004%
8	3.223	676	679	682	rVB2	539	211	0.02%	0.002%
9	3.240	682	684	685	rBV2	690	293	0.02%	0.003%
10	3.346	715	717	719	rBV	429	204	0.02%	0.002%
11	3.362	719	722	724	rVB	638	327	0.02%	0.003%
12	3.400	732	734	737	rVB3	698	301	0.02%	0.003%
13	3.416	737	739	742	rBV	554	343	0.03%	0.003%
14	3.449	746	749	752	rVV3	331	206	0.02%	0.002%
15	3.497	762	764	768	rVB2	437	227	0.02%	0.002%
16	3.532	773	775	780	rVB4	712	386	0.03%	0.004%
17	3.648	807	811	813	rBV4	963	782	0.06%	0.008%
18	3.703	826	828	830	rBV3	589	240	0.02%	0.002%
19	3.728	834	836	839	rBV2	559	322	0.02%	0.003%
20	3.812	859	862	864	rBV2	523	365	0.03%	0.004%
21	3.870	870	880	907	rBV	135434	355606	26.23%	3.498%
22	4.342	1011	1027	1047	rBV	226393	568982	41.98%	5.597%
23	4.645	1120	1121	1122	rBV	556	204	0.02%	0.002%
24	4.866	1188	1190	1196	rVB4	926	692	0.05%	0.007%
25	4.895	1196	1199	1204	rBV7	743	852	0.06%	0.008%
26	4.918	1204	1206	1209	rBV2	550	270	0.02%	0.003%
27	4.976	1222	1224	1227	rBV	408	216	0.02%	0.002%
28	5.040	1227	1244	1264	rBV2	520246	1355465	100.00%	13.333%
29	5.400	1351	1356	1360	rBV6	973	920	0.07%	0.009%
30	5.429	1363	1365	1367	rBV	669	385	0.03%	0.004%
31	5.490	1379	1384	1385	rBV5	937	782	0.06%	0.008%
32	5.522	1391	1394	1396	rBV2	585	341	0.03%	0.003%
33	5.542	1396	1400	1402	rBV3	650	492	0.04%	0.005%
34	5.612	1410	1422	1458	rBV	382593	819843	60.48%	8.064%
35	5.850	1494	1496	1500	rBV5	804	586	0.04%	0.006%
36	5.905	1506	1513	1514	rBV5	4294	4132	0.30%	0.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027272.D
 Acq On : 10 Aug 2022 21:14
 Operator : SY/MD
 Sample : N4144-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	5.979	1533	1536	1539	rBV4	934	550	0.04%	0.005%
38	6.066	1549	1563	1598	rBV	320191	682889	50.38%	6.717%
39	6.288	1630	1632	1634	rBV3	773	327	0.02%	0.003%
40	6.419	1668	1673	1678	rVB5	1205	1242	0.09%	0.012%
41	6.452	1678	1683	1684	rBV3	698	505	0.04%	0.005%
42	6.461	1684	1686	1688	rBV	446	197	0.01%	0.002%
43	6.506	1698	1700	1704	rVB2	739	508	0.04%	0.005%
44	6.538	1707	1710	1712	rBV3	677	468	0.03%	0.005%
45	6.583	1718	1724	1726	rBV5	983	1077	0.08%	0.011%
46	6.715	1763	1765	1770	rVB3	857	483	0.04%	0.005%
47	6.744	1772	1774	1777	rBV3	502	279	0.02%	0.003%
48	6.757	1777	1778	1784	rVB3	491	307	0.02%	0.003%
49	6.805	1790	1793	1797	rBV4	686	506	0.04%	0.005%
50	6.850	1805	1807	1809	rVB2	739	226	0.02%	0.002%
51	6.982	1837	1848	1872	rBV	140220	272218	20.08%	2.678%
52	7.313	1940	1951	1981	rBV	518354	943481	69.61%	9.280%
53	7.619	2036	2046	2070	rBV2	101205	193359	14.27%	1.902%
54	7.934	2142	2144	2147	rVB3	484	234	0.02%	0.002%
55	7.985	2158	2160	2164	rBV4	552	379	0.03%	0.004%
56	8.085	2182	2191	2233	rBV	422186	819082	60.43%	8.057%
57	8.696	2377	2381	2383	rBV4	997	620	0.05%	0.006%
58	8.850	2417	2429	2460	rBV	601683	1008236	74.38%	9.917%
59	9.146	2517	2521	2522	rBV3	1531	1099	0.08%	0.011%
60	9.275	2559	2561	2564	rBV3	758	339	0.03%	0.003%
61	9.287	2564	2565	2567	rBV2	437	200	0.01%	0.002%
62	9.332	2577	2579	2580	rBV2	799	333	0.02%	0.003%
63	9.445	2611	2614	2617	rBV3	434	334	0.02%	0.003%
64	9.538	2636	2643	2645	rBV4	1286	1151	0.08%	0.011%
65	9.564	2650	2651	2654	rVV2	999	486	0.04%	0.005%
66	9.580	2654	2656	2660	rVB4	992	722	0.05%	0.007%
67	9.599	2660	2662	2666	rBV3	847	610	0.05%	0.006%
68	9.632	2670	2672	2675	rVV3	464	341	0.03%	0.003%
69	9.651	2675	2678	2683	rVB3	878	696	0.05%	0.007%
70	9.767	2712	2714	2718	rVB3	512	303	0.02%	0.003%
71	9.796	2721	2723	2726	rBV2	349	232	0.02%	0.002%
72	9.898	2751	2755	2757	rBV3	885	652	0.05%	0.006%
73	9.953	2770	2772	2775	rVB2	556	288	0.02%	0.003%
74	9.985	2778	2782	2785	rBV4	721	474	0.03%	0.005%
75	10.040	2795	2799	2800	rBV2	424	304	0.02%	0.003%
76	10.072	2807	2809	2811	rBV3	543	268	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
 Data File : VV027272.D
 Acq On : 10 Aug 2022 21:14
 Operator : SY/MD
 Sample : N4144-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.107	2817	2820	2823	rBV2	379	311	0.02%	0.003%
78	10.214	2841	2853	2878	rVV	490842	769276	56.75%	7.567%
79	10.339	2890	2892	2895	rVV2	582	222	0.02%	0.002%
80	10.365	2895	2900	2903	rVV4	1033	1001	0.07%	0.010%
81	10.394	2906	2909	2911	rBV4	725	546	0.04%	0.005%
82	10.413	2911	2915	2918	rVB4	956	572	0.04%	0.006%
83	10.455	2924	2928	2934	rVB4	866	792	0.06%	0.008%
84	10.480	2934	2936	2938	rBV	371	198	0.01%	0.002%
85	10.529	2949	2951	2952	rBV	588	272	0.02%	0.003%
86	10.696	3001	3003	3005	rBV3	616	266	0.02%	0.003%
87	10.789	3030	3032	3034	rBV3	398	215	0.02%	0.002%
88	10.869	3055	3057	3061	rVB4	569	345	0.03%	0.003%
89	10.889	3061	3063	3066	rBV2	508	284	0.02%	0.003%
90	10.905	3066	3068	3070	rBV	585	200	0.01%	0.002%
91	11.159	3145	3147	3149	rBV2	592	240	0.02%	0.002%
92	11.249	3163	3175	3193	rBV	491718	785588	57.96%	7.727%
93	11.467	3241	3243	3246	rBV2	755	411	0.03%	0.004%
94	11.622	3280	3291	3312	rBV	521587	821884	60.63%	8.084%
95	11.934	3386	3388	3392	rVB4	1007	496	0.04%	0.005%
96	11.953	3392	3394	3396	rBV3	585	323	0.02%	0.003%
97	12.641	3603	3608	3611	rBV5	738	727	0.05%	0.007%
98	12.680	3618	3620	3623	rBV	626	358	0.03%	0.004%
99	14.229	4100	4102	4106	rVB2	852	348	0.03%	0.003%
100	14.715	4250	4253	4256	rBV2	1085	731	0.05%	0.007%




Sum of corrected areas: 10166383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027272.D
Acq On : 10 Aug 2022 21:14
Operator : SY/MD
Sample : N4144-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

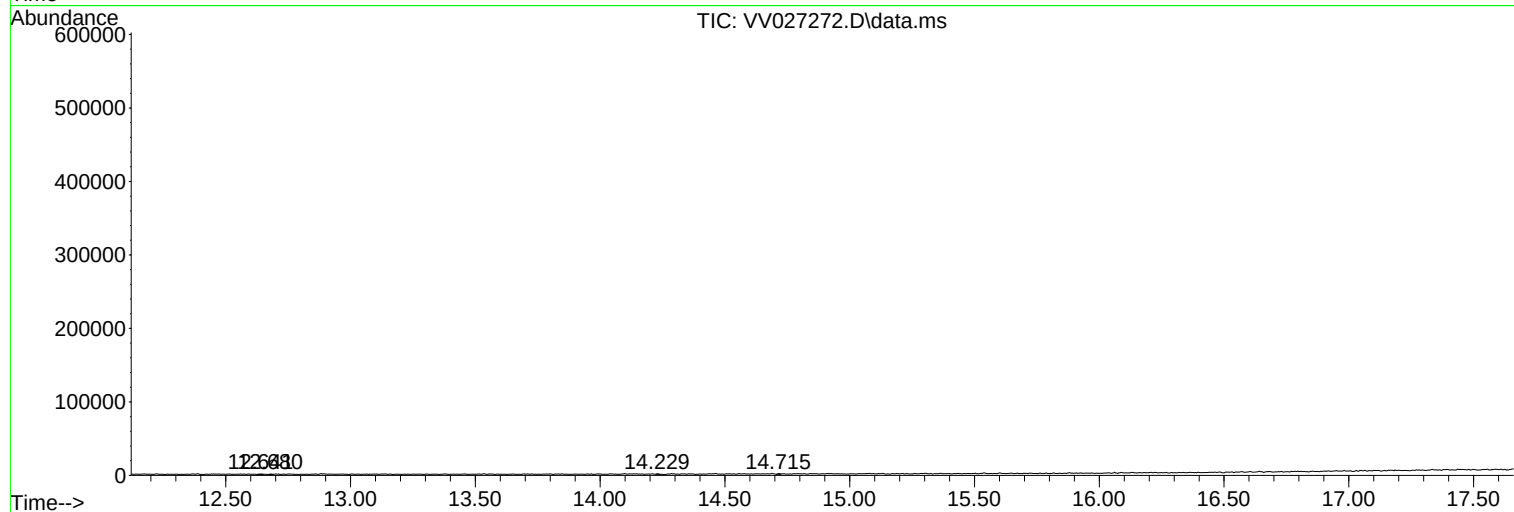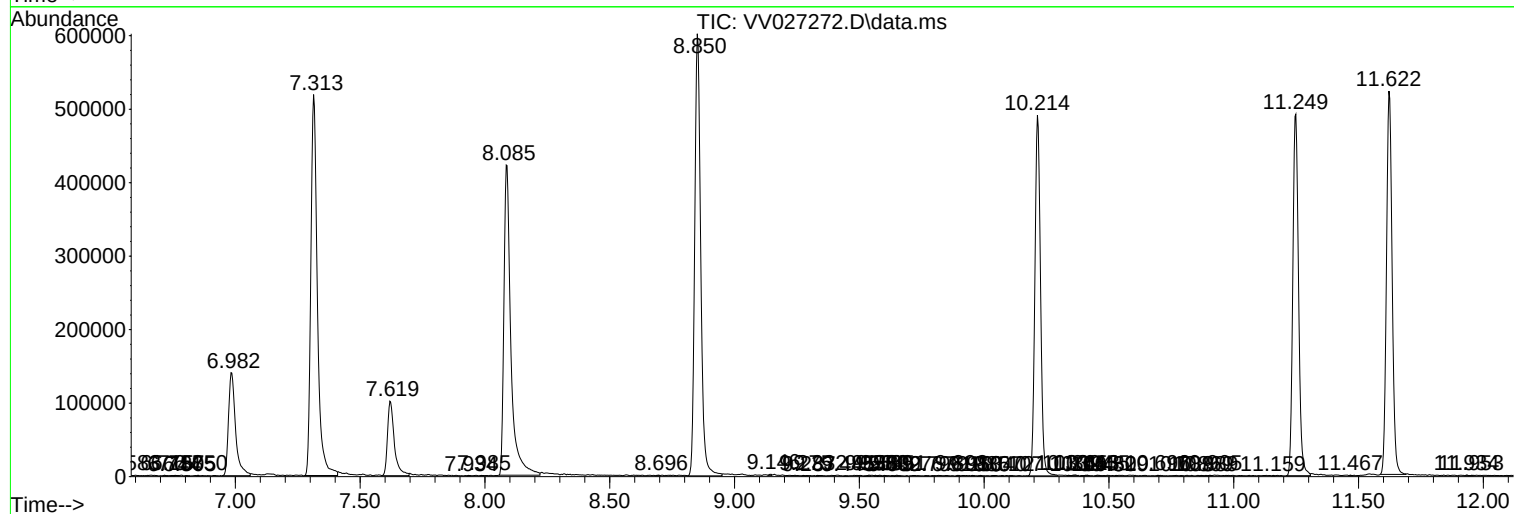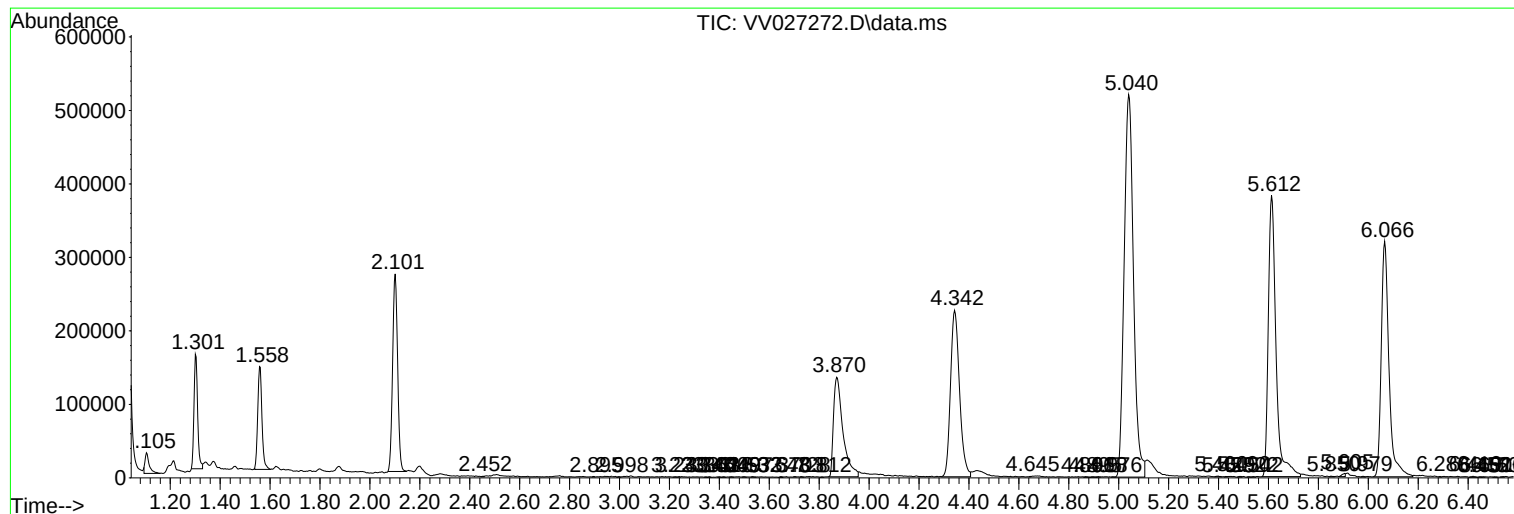

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027272.D
Acq On : 10 Aug 2022 21:14
Operator : SY/MD
Sample : N4144-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081022\
Data File : VV027272.D
Acq On : 10 Aug 2022 21:14
Operator : SY/MD
Sample : N4144-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc