

Data File : VV012189.D
Acq On : 11 Aug 2019 13:35
Operator : SY/MD
Sample : K4248-02DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B05DL

Quant Time: Aug 12 02:34:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Aug 12 01:34:49 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	336196	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	320889	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	156802	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58313	47.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.30%
7) Chloroethane-d5	1.58	69	41912	53.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.28%
11) 1,1-Dichloroethene-d2	2.13	63	81880	35.02	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.04%
21) 2-Butanone-d5	3.93	46	65204	106.62	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.62%
24) Chloroform-d	4.40	84	113733	44.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.52%
26) 1,2-Dichloroethane-d4	5.08	65	70448	47.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.62%
32) Benzene-d6	5.10	84	236149	47.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.94%
36) 1,2-Dichloropropane-d6	6.12	67	63413	46.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.72%
41) Toluene-d8	7.36	98	213617	45.07	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.14%
43) trans-1,3-Dichloropropene-	7.66	79	31719	43.25	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.50%
47) 2-Hexanone-d5	8.13	63	45658	88.18	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.18%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	85384	46.02	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.04%
64) 1,2-Dichlorobenzene-d4	11.67	152	86980	46.93	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.86%

Target Compounds


					Qvalue
5) Vinyl chloride	1.32	62	9230	4.966 ug/L	# 76
17) trans-1,2-Dichloroethene	2.80	96	3634	1.826 ug/L	76
20) cis-1,2-Dichloroethene	3.96	96	81350	35.983 ug/L	97
34) Trichloroethene	5.96	95	27220	12.295 ug/L	98
46) Tetrachloroethene	8.02	164	16232	7.670 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV012189.D
Acq On : 11 Aug 2019 13:35
Operator : SY/MD
Sample : K4248-02DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B05DL

Quant Time: Aug 12 02:34:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Aug 12 01:34:49 2019
Response via : Initial Calibration

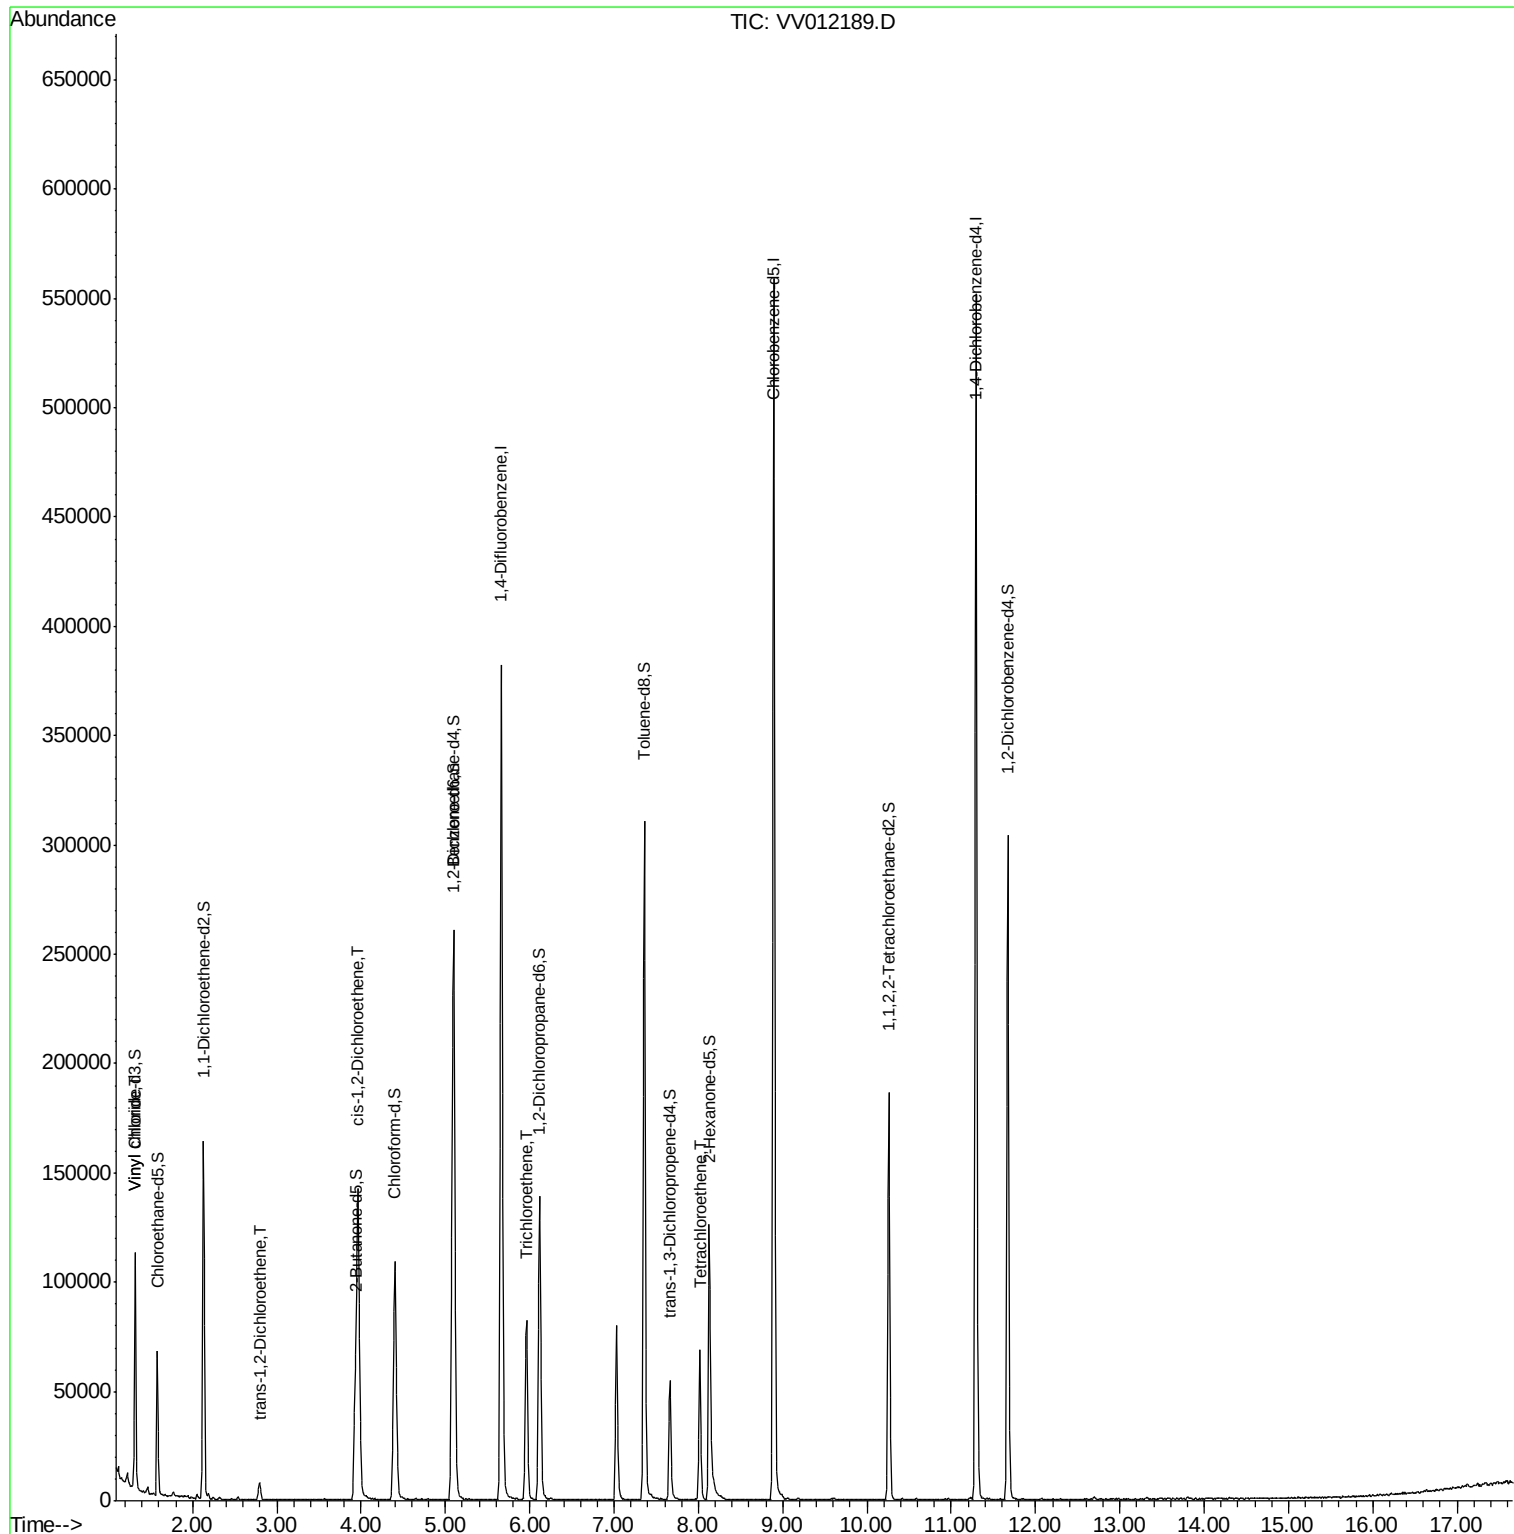

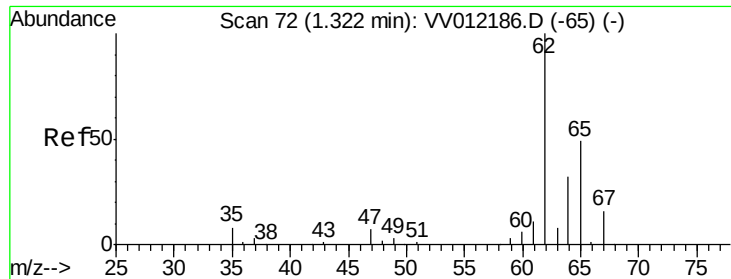

#5

Vinyl chloride

Concen: 4.966 ug/L

RT: 1.32 min Scan# 72

Delta R.T. 0.00 min

Lab File: VV012189.D

Acq: 11 Aug 2019 13:35

Instrument :

MSVOA_V

ClientSampled :





F2B05DL

Tgt Ion: 62 Resp: 9230

Ion Ratio Lower Upper

62 100

64 47.4 23.7 44.1#

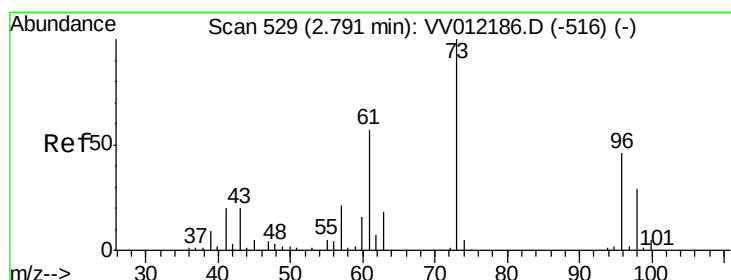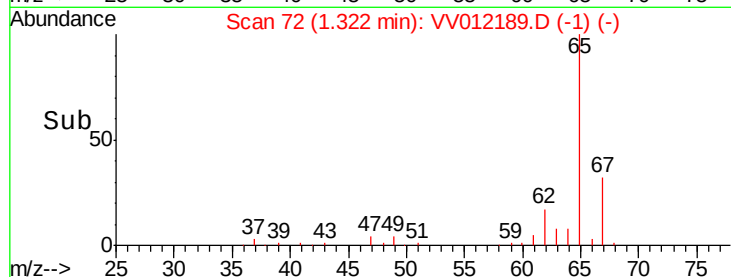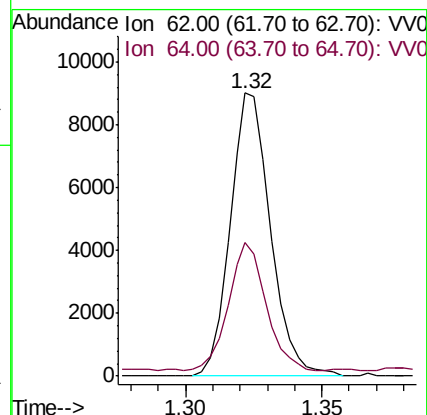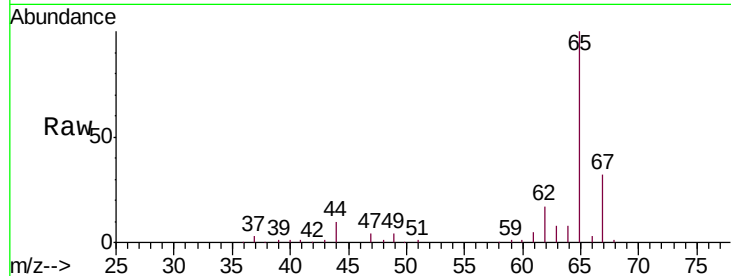

#17

trans-1,2-Dichloroethene

Concen: 1.826 ug/L

RT: 2.80 min Scan# 531

Delta R.T. 0.01 min

Lab File: VV012189.D

Acq: 11 Aug 2019 13:35




Tgt Ion: 96 Resp: 3634


Ion Ratio Lower Upper

96 100

61 96.7 89.3 165.9

98 49.7 44.7 83.1

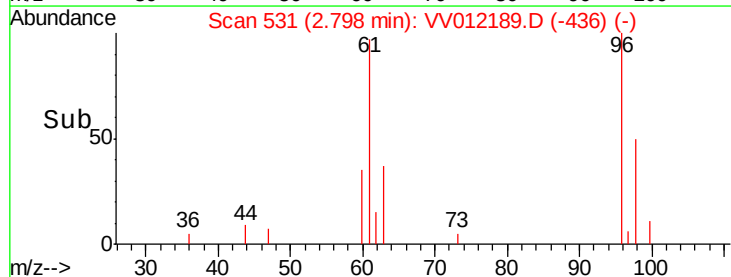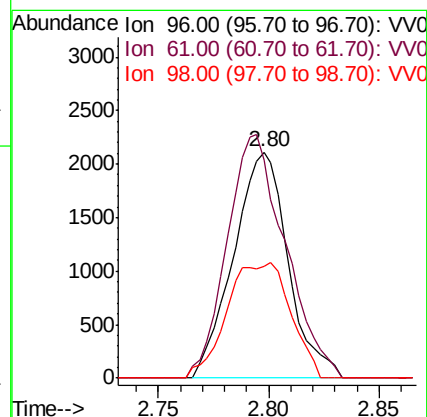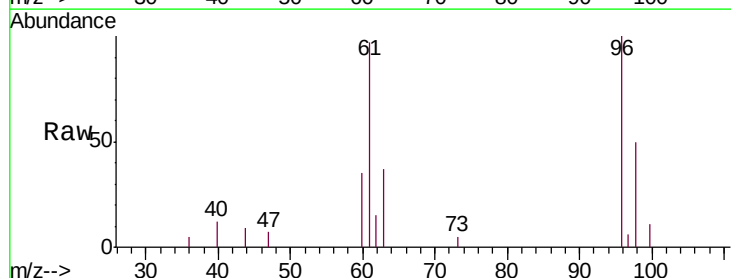




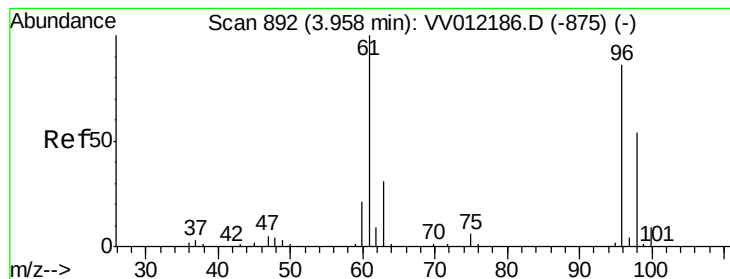


#20

cis-1,2-Dichloroethene
 Concen: 35.983 ug/L
 RT: 3.96 min Scan# 894
 Delta R.T. 0.01 min
 Lab File: VV012189.D
 Acq: 11 Aug 2019 13:35

Instrument :
 MSVOA_V
 ClientSampled :
 F2B05DL




Tgt Ion: 96 Resp: 81350
 Ion Ratio Lower Upper
 96 100
 61 115.1 82.9 153.9
 68 0.0 0.0 0.0

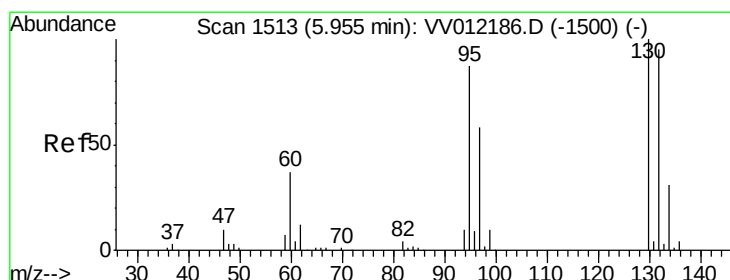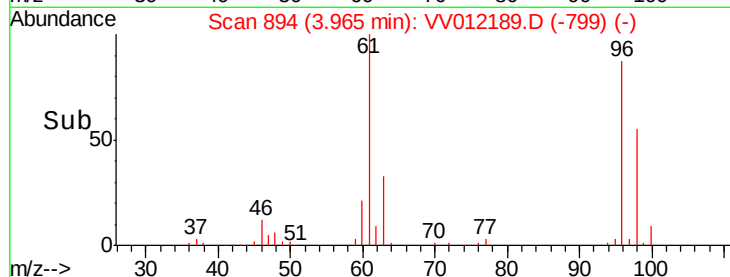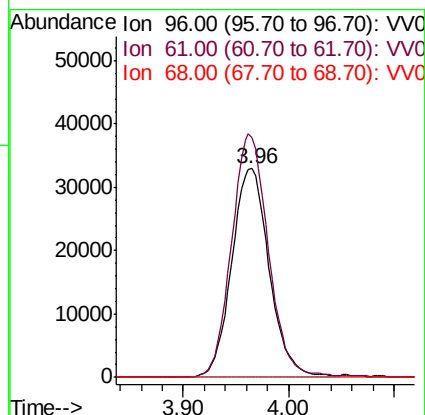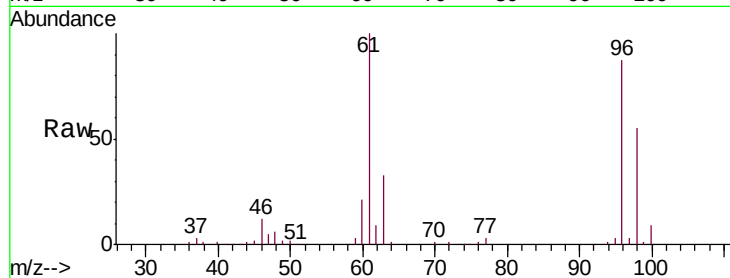


#34

Trichloroethene
 Concen: 12.295 ug/L
 RT: 5.96 min Scan# 1514
 Delta R.T. 0.00 min
 Lab File: VV012189.D
 Acq: 11 Aug 2019 13:35

Tgt Ion: 95 Resp: 27220
 Ion Ratio Lower Upper
 95 100
 97 63.2 44.7 83.1
 132 108.0 72.7 134.9
 130 110.4 75.9 141.1

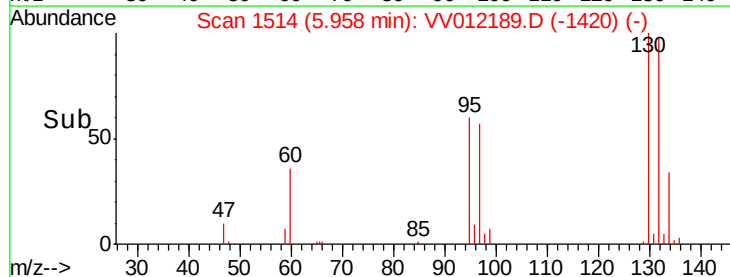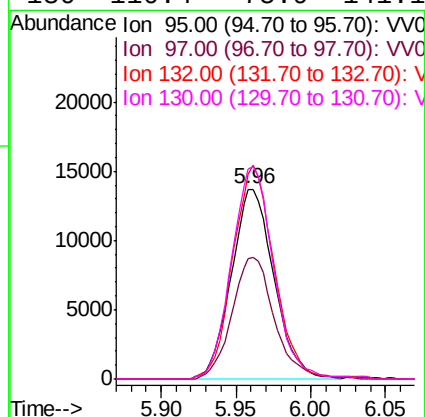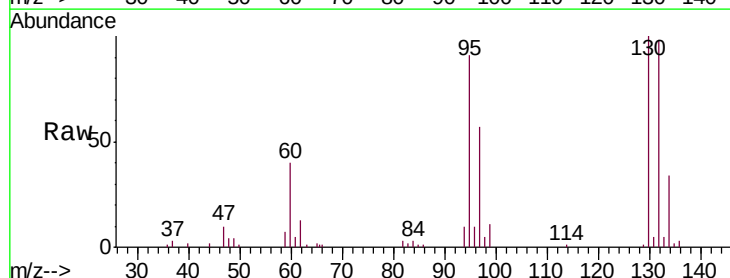

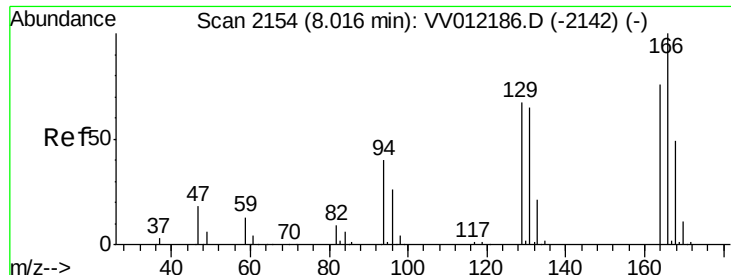

#46

Tetrachloroethene

Concen: 7.670 ug/L

RT: 8.02 min Scan# 2154

Delta R.T. 0.00 min

Lab File: VV012189.D

Acq: 11 Aug 2019 13:35

Instrument :
MSVOA_V
ClientSampleId :
F2B05DL

Tgt Ion:164 Resp: 16232



Ion Ratio Lower Upper

164 100

129 88.1 60.6 112.6

131 82.2 59.5 110.5

166 127.6 87.2 161.9

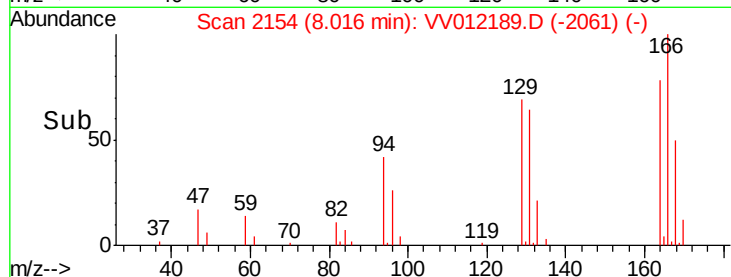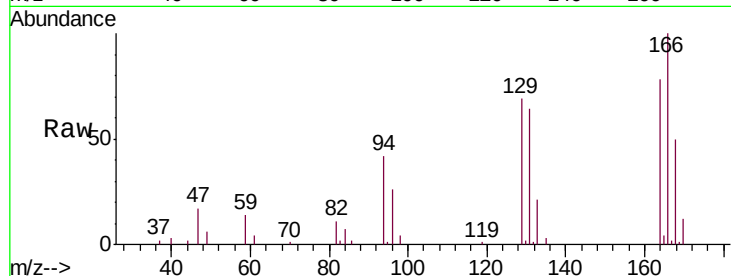

Abundance Ion 164.00 (163.70 to 164.70): V
Ion 129.00 (128.70 to 129.70): V
Ion 131.00 (130.70 to 131.70): V
Ion 166.00 (165.70 to 166.70): V

