

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
 Data File : VV012189.D
 Acq On : 11 Aug 2019 13:35
 Operator : SY/MD
 Sample : K4248-02DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B05DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	86	rVB2	108543	116868	12.87%	1.736%
2	1.582	146	153	171	rVB	66141	78199	8.61%	1.161%
3	2.055	294	300	307	rBV4	2269	2980	0.33%	0.044%
4	2.084	307	309	310	rBV2	450	142	0.02%	0.002%
5	2.129	313	323	335	rBV	163499	230981	25.43%	3.431%
6	2.467	423	428	433	rVB3	467	481	0.05%	0.007%
7	2.537	444	450	455	rVB4	1020	1468	0.16%	0.022%
8	2.663	486	489	491	rBV2	301	210	0.02%	0.003%
9	2.795	521	530	542	rVB3	7821	14131	1.56%	0.210%
10	2.952	576	579	582	rBV2	174	101	0.01%	0.002%
11	3.042	605	607	611	rBV2	163	105	0.01%	0.002%
12	3.431	727	728	730	rVB	273	56	0.01%	0.001%
13	3.450	730	734	736	rBV2	185	146	0.02%	0.002%
14	3.496	745	748	749	rBV2	162	86	0.01%	0.001%
15	3.537	758	761	765	rVB	235	148	0.02%	0.002%
16	3.553	765	766	767	rBV	212	75	0.01%	0.001%
17	3.563	767	769	770	rVB	542	132	0.01%	0.002%
18	3.711	812	815	818	rBV2	236	169	0.02%	0.003%
19	3.791	835	840	844	rBV2	288	384	0.04%	0.006%
20	3.856	857	860	863	rBV	145	97	0.01%	0.001%
21	3.962	870	893	920	rBV3	142686	435895	47.99%	6.474%
22	4.219	966	973	975	rBV	366	368	0.04%	0.005%
23	4.399	1013	1029	1051	rBV2	108845	266363	29.33%	3.956%
24	4.595	1087	1090	1093	rBV2	379	302	0.03%	0.004%
25	4.653	1104	1108	1110	rBV3	353	235	0.03%	0.003%
26	4.743	1131	1136	1137	rBV2	288	195	0.02%	0.003%
27	4.872	1173	1176	1178	rBV	370	223	0.02%	0.003%
28	4.939	1195	1197	1200	rBV2	241	129	0.01%	0.002%
29	4.978	1205	1209	1210	rBV	118	82	0.01%	0.001%
30	5.010	1217	1219	1221	rBV2	176	77	0.01%	0.001%
31	5.097	1227	1246	1273	rBV2	260861	654381	72.04%	9.720%
32	5.348	1322	1324	1327	rVB	191	102	0.01%	0.002%
33	5.447	1352	1355	1357	rBV	284	146	0.02%	0.002%
34	5.473	1361	1363	1368	rVB2	174	102	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
 Data File : VV012189.D
 Acq On : 11 Aug 2019 13:35
 Operator : SY/MD
 Sample : K4248-02DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B05DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

35	5.502	1369	1372	1373	rBV2	160	80	0.01%	0.001%
36	5.508	1373	1374	1378	rBV	250	149	0.02%	0.002%
37	5.602	1399	1403	1407	rVB2	295	254	0.03%	0.004%
38	5.663	1407	1422	1451	rBV	382116	752115	82.80%	11.171%
39	5.962	1501	1515	1533	rBV	81466	158513	17.45%	2.354%
40	6.116	1549	1563	1588	rBV	138534	279174	30.74%	4.147%
41	6.280	1610	1614	1618	rBV2	370	235	0.03%	0.003%
42	6.479	1672	1676	1679	rBV2	267	172	0.02%	0.003%
43	6.528	1689	1691	1693	rBV	307	132	0.01%	0.002%
44	6.544	1694	1696	1697	rVV2	165	48	0.01%	0.001%
45	6.666	1729	1734	1735	rBV2	362	252	0.03%	0.004%
46	6.688	1739	1741	1744	rBV2	236	169	0.02%	0.003%
47	6.785	1769	1771	1772	rBV	174	42	0.00%	0.001%
48	6.881	1798	1801	1804	rBV	310	296	0.03%	0.004%
49	6.894	1804	1805	1807	rVB	222	95	0.01%	0.001%
50	7.029	1836	1847	1870	rBV	79579	144475	15.91%	2.146%
51	7.174	1890	1892	1896	rVB2	248	143	0.02%	0.002%
52	7.196	1896	1899	1901	rBV2	398	202	0.02%	0.003%
53	7.360	1936	1950	1967	rBV	310243	543433	59.83%	8.072%
54	7.611	2025	2028	2033	rVB	301	208	0.02%	0.003%
55	7.663	2033	2044	2070	rBV	54758	96008	10.57%	1.426%
56	7.820	2091	2093	2095	rBV	236	132	0.01%	0.002%
57	7.830	2095	2096	2097	rVB	410	80	0.01%	0.001%
58	7.849	2100	2102	2104	rVB2	230	81	0.01%	0.001%
59	7.884	2110	2113	2115	rBV2	410	251	0.03%	0.004%
60	7.939	2128	2130	2135	rBV2	265	271	0.03%	0.004%
61	8.019	2143	2155	2171	rVB2	68701	114434	12.60%	1.700%
62	8.129	2179	2189	2217	rBV	125916	243238	26.78%	3.613%
63	8.392	2269	2271	2273	rBV	148	49	0.01%	0.001%
64	8.444	2284	2287	2293	rVB2	240	154	0.02%	0.002%
65	8.576	2326	2328	2333	rVB2	215	132	0.01%	0.002%
66	8.608	2333	2338	2340	rBV2	319	284	0.03%	0.004%
67	8.894	2414	2427	2453	rBV	558576	908298	100.00%	13.491%
68	9.097	2489	2490	2493	rBV	272	77	0.01%	0.001%
69	9.331	2560	2563	2565	rBV2	260	177	0.02%	0.003%
70	9.415	2585	2589	2594	rBV2	155	173	0.02%	0.003%
71	9.585	2638	2642	2645	rBV3	442	380	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
 Data File : VV012189.D
 Acq On : 11 Aug 2019 13:35
 Operator : SY/MD
 Sample : K4248-02DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B05DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

72	9.605	2645	2648	2650	rBV2	500	371	0.04%	0.006%
73	9.662	2662	2666	2668	rBV	255	187	0.02%	0.003%
74	9.746	2688	2692	2696	rBV2	225	242	0.03%	0.004%
75	9.839	2716	2721	2722	rBV	233	185	0.02%	0.003%
76	9.949	2754	2755	2756	rBV	162	31	0.00%	0.000%
77	9.974	2756	2763	2769	rVB3	381	597	0.07%	0.009%
78	10.003	2769	2772	2773	rBV	174	83	0.01%	0.001%
79	10.074	2791	2794	2796	rBV	264	187	0.02%	0.003%
80	10.261	2840	2852	2872	rBV	185979	296818	32.68%	4.409%
81	10.534	2934	2937	2940	rBV2	287	165	0.02%	0.002%
82	10.759	3005	3007	3009	rBV	305	79	0.01%	0.001%
83	10.907	3051	3053	3056	rVB	315	142	0.02%	0.002%
84	10.933	3058	3061	3063	rVV	458	195	0.02%	0.003%
85	11.129	3119	3122	3126	rBV2	269	214	0.02%	0.003%
86	11.228	3143	3153	3161	rBV5	1214	1797	0.20%	0.027%
87	11.293	3161	3173	3195	rBV	551195	884911	97.43%	13.144%
88	11.669	3278	3290	3309	rBV	303702	492701	54.24%	7.318%
89	11.855	3346	3348	3351	rVB	564	186	0.02%	0.003%
90	12.209	3457	3458	3459	rBV	270	55	0.01%	0.001%
91	12.695	3603	3609	3614	rBV3	1301	1633	0.18%	0.024%
92	12.785	3634	3637	3639	rBV2	317	190	0.02%	0.003%
93	12.949	3687	3688	3689	rBV	332	81	0.01%	0.001%
94	13.669	3909	3912	3914	rBV	523	309	0.03%	0.005%
95	13.801	3947	3953	3958	rBV3	777	1175	0.13%	0.017%
96	14.302	4107	4109	4110	rBV	561	126	0.01%	0.002%


Sum of corrected areas: 6732625

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
Data File : VV012189.D
Acq On : 11 Aug 2019 13:35
Operator : SY/MD
Sample : K4248-02DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B05DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

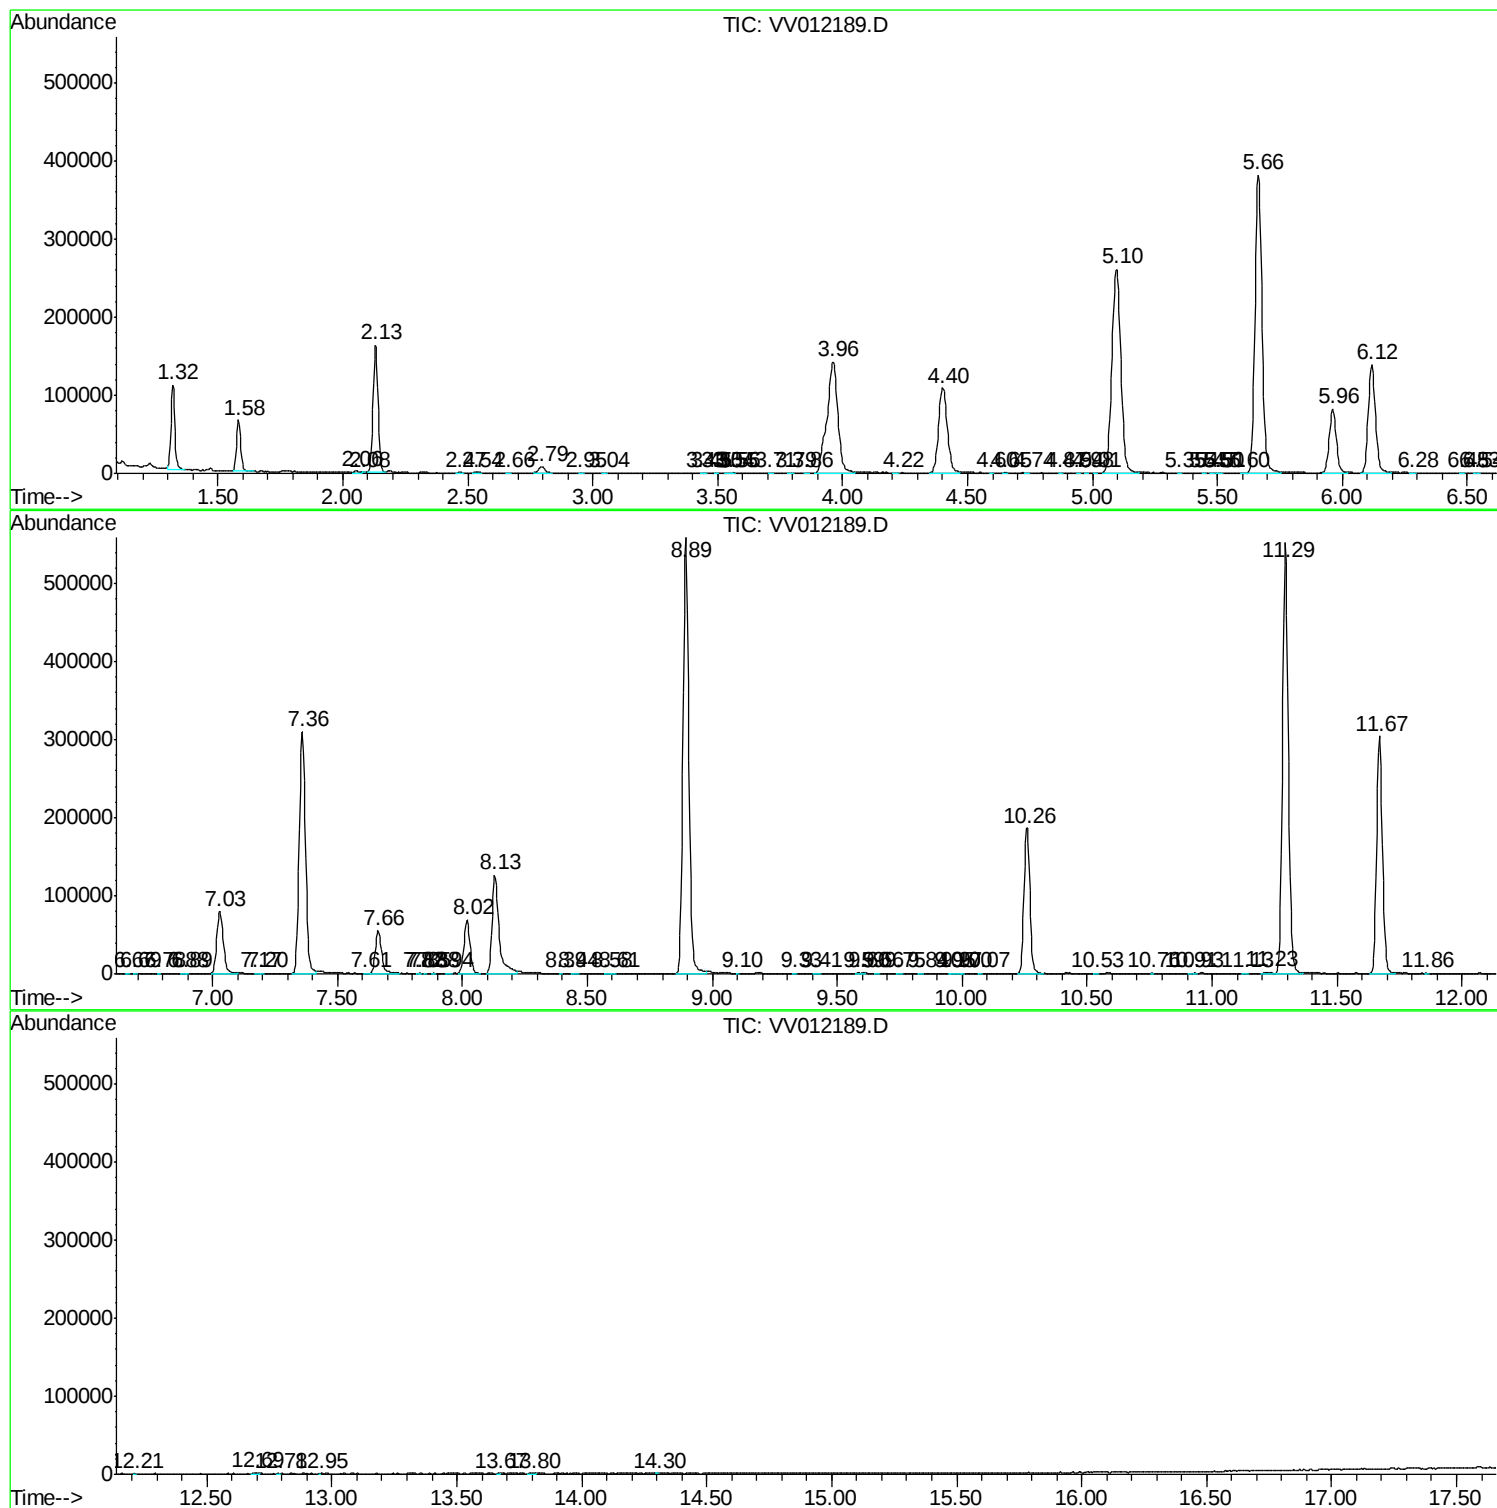

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
Data File : VV012189.D
Acq On : 11 Aug 2019 13:35
Operator : SY/MD
Sample : K4248-02DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B05DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
Data File : VV012189.D
Acq On : 11 Aug 2019 13:35
Operator : SY/MD
Sample : K4248-02DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B05DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc