

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
 Data File : VV012190.D
 Acq On : 11 Aug 2019 13:58
 Operator : SY/MD
 Sample : K4248-03DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B06DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	83	rVB	110345	116576	12.74%	1.714%
2	1.582	145	153	164	rBV	68201	77148	8.43%	1.135%
3	1.975	271	275	280	rBV5	968	1229	0.13%	0.018%
4	2.036	291	294	295	rBV3	571	306	0.03%	0.005%
5	2.129	312	323	335	rBV	171590	242355	26.49%	3.564%
6	2.241	354	358	359	rBV2	542	470	0.05%	0.007%
7	2.422	411	414	417	rBV2	283	185	0.02%	0.003%
8	2.463	424	427	429	rBV2	350	204	0.02%	0.003%
9	2.534	441	449	457	rBV4	996	1446	0.16%	0.021%
10	2.573	457	461	465	rBV	222	215	0.02%	0.003%
11	2.795	519	530	541	rBV6	5565	10626	1.16%	0.156%
12	2.894	559	561	566	rVB2	257	191	0.02%	0.003%
13	2.920	566	569	573	rBV2	280	274	0.03%	0.004%
14	2.981	583	588	590	rBV	288	194	0.02%	0.003%
15	3.547	761	764	767	rBV2	266	212	0.02%	0.003%
16	3.730	817	821	824	rBV2	262	203	0.02%	0.003%
17	3.823	847	850	856	rVB2	245	242	0.03%	0.004%
18	3.962	870	893	917	rBV2	116400	380315	41.56%	5.593%
19	4.148	946	951	955	rBV4	615	462	0.05%	0.007%
20	4.399	1012	1029	1052	rVV2	111940	274124	29.96%	4.031%
21	4.547	1073	1075	1078	rBV2	518	274	0.03%	0.004%
22	4.672	1111	1114	1118	rBV2	222	211	0.02%	0.003%
23	4.778	1145	1147	1153	rVB3	258	198	0.02%	0.003%
24	4.904	1182	1186	1191	rBV2	242	282	0.03%	0.004%
25	5.093	1228	1245	1270	rBV3	270061	673355	73.59%	9.903%
26	5.286	1303	1305	1311	rVB3	284	256	0.03%	0.004%
27	5.450	1354	1356	1362	rVB3	295	202	0.02%	0.003%
28	5.563	1388	1391	1394	rBV2	433	280	0.03%	0.004%
29	5.663	1408	1422	1443	rBV	379804	747015	81.64%	10.986%
30	5.836	1473	1476	1478	rBV2	392	255	0.03%	0.004%
31	5.862	1482	1484	1493	rVB2	510	476	0.05%	0.007%
32	5.958	1498	1514	1535	rBV	136579	271525	29.67%	3.993%
33	6.116	1548	1563	1588	rBV	145654	293733	32.10%	4.320%
34	6.238	1596	1601	1607	rBV3	509	495	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
 Data File : VV012190.D
 Acq On : 11 Aug 2019 13:58
 Operator : SY/MD
 Sample : K4248-03DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B06DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

35	6.502	1681	1683	1687	rVB	377	242	0.03%	0.004%
36	6.531	1687	1692	1695	rBV2	307	336	0.04%	0.005%
37	6.717	1745	1750	1752	rBV2	314	290	0.03%	0.004%
38	7.029	1834	1847	1867	rBV	83521	148624	16.24%	2.186%
39	7.145	1880	1883	1887	rVV4	282	219	0.02%	0.003%
40	7.228	1906	1909	1913	rBV	187	194	0.02%	0.003%
41	7.251	1913	1916	1923	rVB2	298	226	0.02%	0.003%
42	7.309	1930	1934	1935	rBV	338	218	0.02%	0.003%
43	7.360	1936	1950	1968	rBV	327770	559015	61.09%	8.221%
44	7.589	2018	2021	2026	rBV4	307	261	0.03%	0.004%
45	7.617	2026	2030	2033	rBV2	232	223	0.02%	0.003%
46	7.662	2033	2044	2065	rVV	57792	98936	10.81%	1.455%
47	7.756	2070	2073	2076	rBV3	307	252	0.03%	0.004%
48	7.929	2124	2127	2129	rBV2	294	218	0.02%	0.003%
49	7.981	2136	2143	2146	rBV3	550	709	0.08%	0.010%
50	8.019	2146	2155	2167	rVB2	15440	25042	2.74%	0.368%
51	8.129	2178	2189	2217	rBV	130749	250227	27.35%	3.680%
52	8.344	2253	2256	2261	rVB3	486	469	0.05%	0.007%
53	8.373	2262	2265	2267	rBV	383	222	0.02%	0.003%
54	8.405	2271	2275	2281	rVB2	412	484	0.05%	0.007%
55	8.460	2288	2292	2299	rVB2	359	360	0.04%	0.005%
56	8.569	2323	2326	2331	rBV	234	208	0.02%	0.003%
57	8.765	2384	2387	2392	rBV	224	208	0.02%	0.003%
58	8.894	2414	2427	2462	rBV	550893	915056	100.00%	13.457%
59	9.055	2471	2477	2480	rBV3	697	633	0.07%	0.009%
60	9.093	2485	2489	2495	rVB2	483	489	0.05%	0.007%
61	9.132	2495	2501	2503	rBV2	401	387	0.04%	0.006%
62	9.183	2512	2517	2520	rBV2	571	448	0.05%	0.007%
63	9.283	2545	2548	2554	rBV2	186	219	0.02%	0.003%
64	9.585	2636	2642	2646	rBV4	681	558	0.06%	0.008%
65	9.614	2648	2651	2657	rVB4	497	357	0.04%	0.005%
66	9.695	2671	2676	2680	rBV2	238	256	0.03%	0.004%
67	10.260	2840	2852	2874	rVB	188686	302842	33.10%	4.454%
68	10.360	2879	2883	2888	rBV2	251	259	0.03%	0.004%
69	10.431	2902	2905	2910	rVB2	286	257	0.03%	0.004%
70	10.617	2961	2963	2971	rVB2	264	205	0.02%	0.003%
71	10.884	3043	3046	3051	rVB2	243	206	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
 Data File : VV012190.D
 Acq On : 11 Aug 2019 13:58
 Operator : SY/MD
 Sample : K4248-03DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B06DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis

72	10.958	3066	3069	3075	rVB2	566	495	0.05%	0.007%
73	11.219	3144	3150	3160	rBV5	1207	1959	0.21%	0.029%
74	11.293	3160	3173	3193	rBV	542179	880033	96.17%	12.942%
75	11.469	3226	3228	3232	rVB2	372	218	0.02%	0.003%
76	11.669	3277	3290	3310	rBV	312609	503471	55.02%	7.404%
77	11.791	3326	3328	3334	rBV2	351	307	0.03%	0.005%
78	11.910	3362	3365	3368	rBV	273	229	0.03%	0.003%
79	12.080	3415	3418	3423	rVB2	337	240	0.03%	0.004%
80	12.141	3432	3437	3439	rBV	298	244	0.03%	0.004%
81	12.212	3453	3459	3463	rBV3	373	436	0.05%	0.006%
82	12.505	3544	3550	3556	rBV2	394	498	0.05%	0.007%
83	12.547	3561	3563	3569	rBV	318	311	0.03%	0.005%
84	12.624	3584	3587	3594	rVB3	330	301	0.03%	0.004%
85	12.662	3596	3599	3603	rVB2	351	205	0.02%	0.003%
86	12.691	3603	3608	3609	rBV	1002	652	0.07%	0.010%
87	12.833	3648	3652	3655	rBV2	287	226	0.02%	0.003%
88	12.887	3666	3669	3673	rBV2	324	209	0.02%	0.003%
89	12.981	3696	3698	3702	rBV2	334	279	0.03%	0.004%
90	13.003	3703	3705	3712	rVB2	514	355	0.04%	0.005%
91	13.196	3760	3765	3767	rBV	302	276	0.03%	0.004%
92	13.566	3875	3880	3884	rBV3	451	504	0.06%	0.007%
93	13.852	3966	3969	3971	rBV2	326	239	0.03%	0.004%
94	13.958	3999	4002	4005	rBV2	540	337	0.04%	0.005%
95	14.087	4038	4042	4046	rVB3	405	362	0.04%	0.005%
96	14.193	4071	4075	4079	rBV2	381	368	0.04%	0.005%
97	14.993	4320	4324	4327	rBV2	637	504	0.06%	0.007%
98	15.103	4356	4358	4361	rBV2	350	198	0.02%	0.003%
99	15.350	4433	4435	4440	rBV	475	415	0.05%	0.006%
100	15.492	4475	4479	4484	rBV5	796	864	0.09%	0.013%


Sum of corrected areas: 6799624

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
Data File : VV012190.D
Acq On : 11 Aug 2019 13:58
Operator : SY/MD
Sample : K4248-03DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B06DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

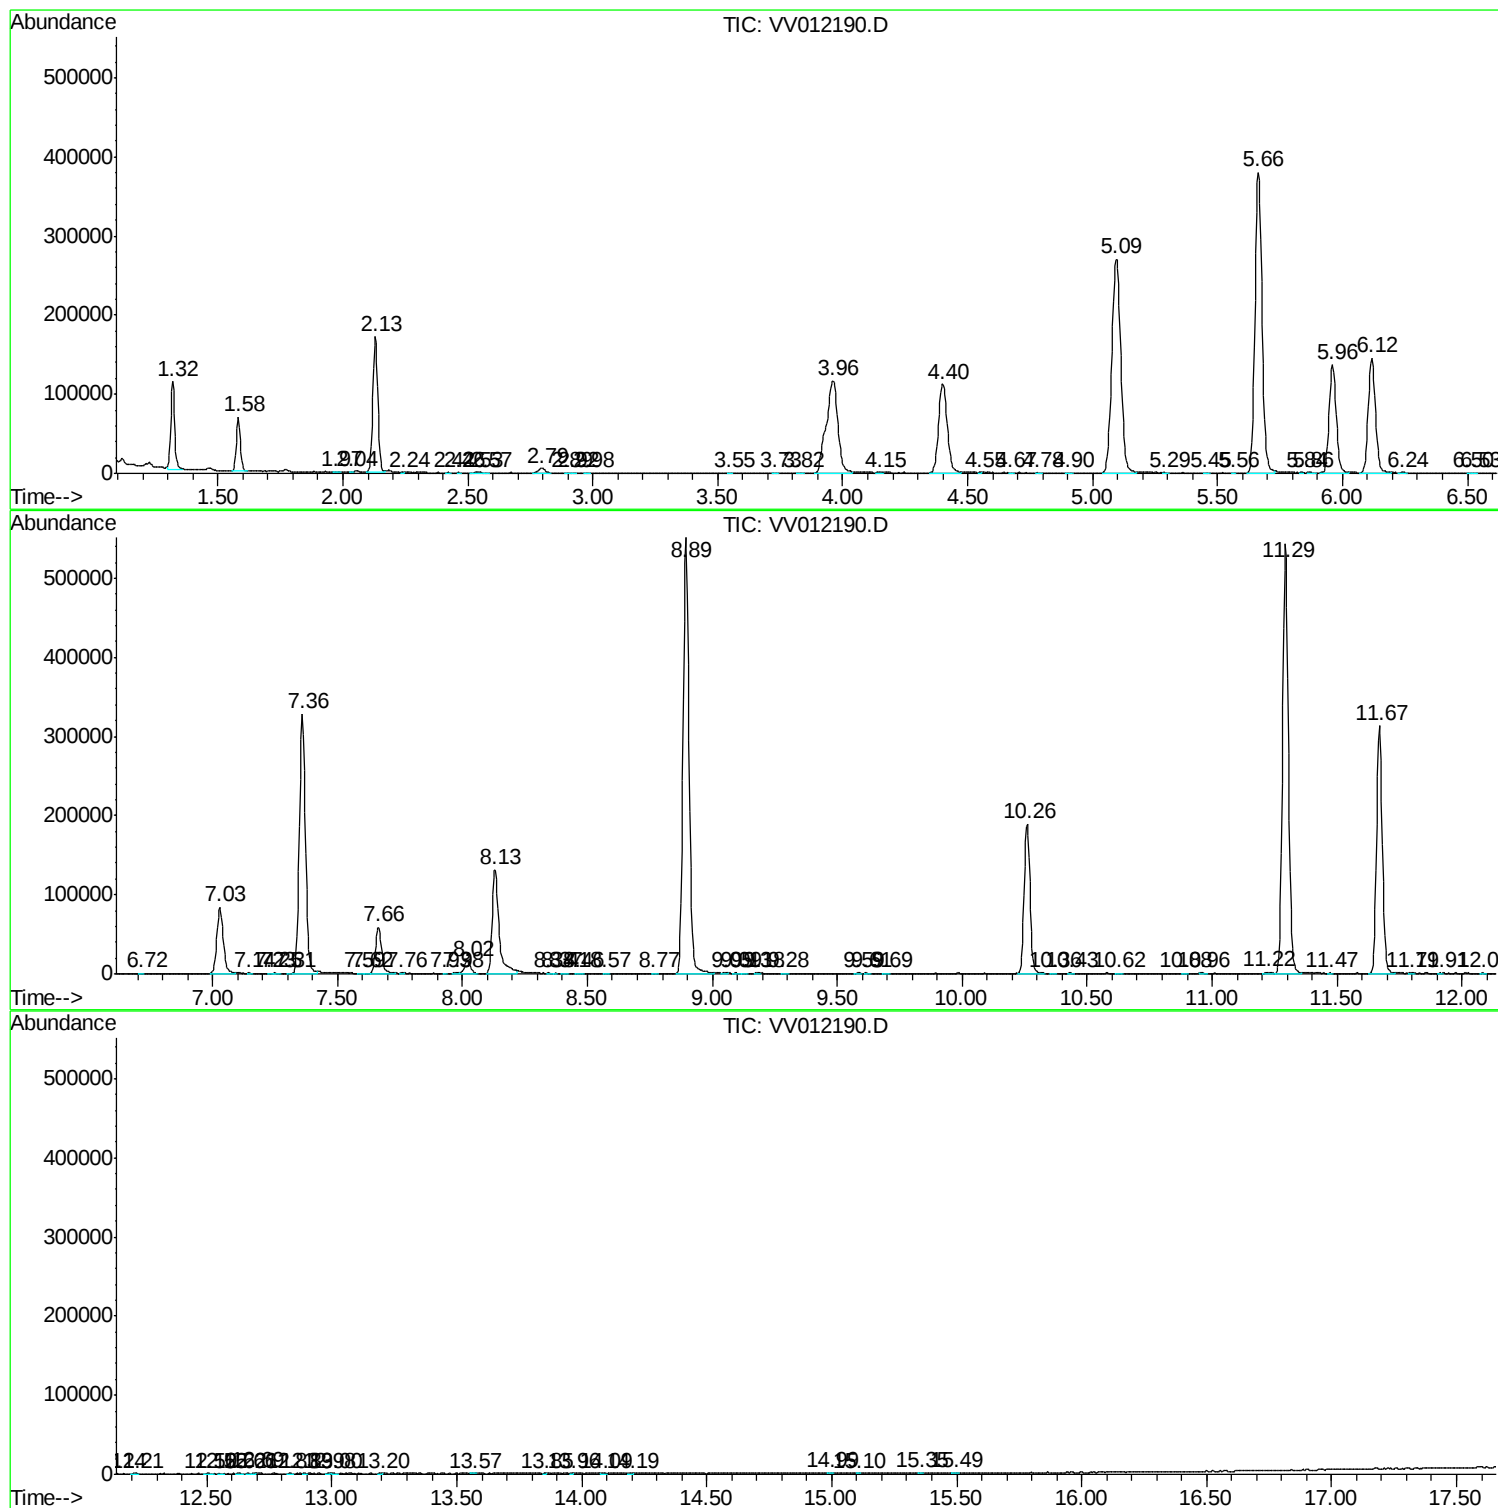

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
Data File : VV012190.D
Acq On : 11 Aug 2019 13:58
Operator : SY/MD
Sample : K4248-03DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B06DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV081119\
Data File : VV012190.D
Acq On : 11 Aug 2019 13:58
Operator : SY/MD
Sample : K4248-03DL 40X
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F2B06DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM081019WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc