


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081119\
 Data File : VV012185.D
 Acq On : 11 Aug 2019 08:46
 Operator : SY/MD
 Sample : BFB64
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081019WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 12 19:05:41 2019

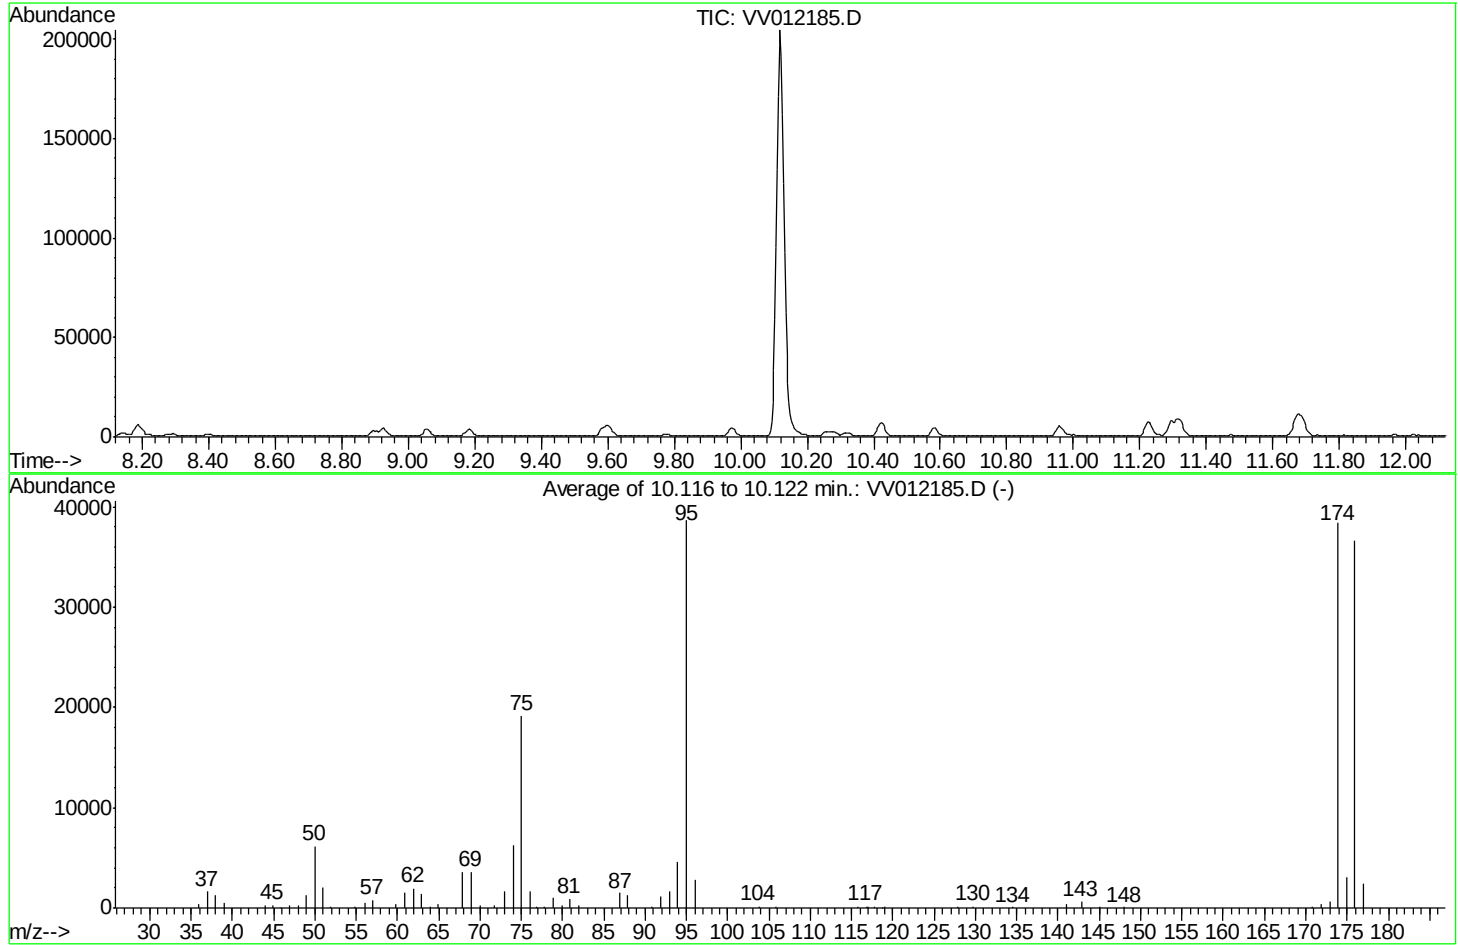

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	6135	PASS
75	95	30	80	49.6	19178	PASS
95	95	100	100	100.0	38680	PASS
96	95	5	9	7.3	2834	PASS
173	174	0.00	2	1.6	612	PASS
174	95	50	120	99.3	38402	PASS
175	174	5	9	8.0	3063	PASS
176	174	95	101	95.4	36645	PASS
177	176	5	9	6.5	2385	PASS

m/z	Abundance
35.90	420.0
37.00	1550.0
38.00	1389.0
39.10	515.0
39.90	285.0
44.00	447.0
44.90	284.0
46.90	304.0
48.00	192.0
49.00	1347.0
50.00	6265.0
51.00	2168.0
51.90	131.0
54.90	103.0
56.00	411.0
57.00	807.0
59.90	364.0
60.90	1603.0
61.90	1954.0
62.90	1510.0
63.90	149.0
64.90	298.0
67.90	3383.0
68.90	3767.0
70.00	319.0
71.70	291.0
73.00	1724.0
74.00	6278.0
75.00	19408.0
76.00	1579.0
76.80	185.0
77.70	142.0
78.90	1068.0
80.00	277.0
80.80	960.0
81.90	194.0
86.90	1432.0
87.80	1122.0
90.80	197.0
91.90	1153.0
93.00	1718.0
93.90	4725.0
95.00	39336.0
96.00	2887.0
103.80	188.0
105.90	178.0
115.80	127.0
116.80	302.0
118.70	161.0
129.80	171.0
134.60	111.0
140.90	468.0
142.80	586.0
145.00	152.0
148.00	162.0
171.90	400.0
173.00	570.0
173.90	37272.0
174.90	3016.0
175.90	36160.0
176.90	2487.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
39.90	306.0
43.90	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	336.0
36.90	1643.0
38.00	1159.0
39.00	489.0
39.90	319.0
44.00	376.0
44.80	274.0
46.90	297.0
47.90	208.0
49.00	1147.0
50.00	5851.0
51.00	1964.0
51.90	117.0
54.80	142.0
56.00	522.0
57.00	752.0
59.80	374.0
60.90	1373.0
62.00	1851.0
63.00	1376.0
63.90	184.0
64.90	348.0
67.90	3598.0
68.90	3340.0
70.00	300.0
71.80	152.0
73.00	1481.0
74.00	5970.0
75.00	18288.0
76.00	1659.0
76.80	193.0
77.80	151.0
78.80	979.0
79.90	272.0
80.80	934.0
82.00	197.0
87.00	1542.0
87.80	1303.0
90.90	155.0
91.90	1086.0
93.00	1570.0
94.00	4454.0
95.00	36752.0
96.00	2673.0
103.80	186.0
105.90	181.0
115.80	170.0
117.00	234.0
117.70	154.0
118.90	205.0
127.80	196.0
129.70	136.0
134.50	105.0
140.90	391.0
142.80	571.0
170.70	123.0
171.80	454.0
172.90	601.0
173.90	38200.0
174.90	2990.0
175.90	35744.0
176.90	2256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
35.90	401.0
36.90	1706.0
38.00	1376.0
39.10	514.0
39.90	308.0
44.00	434.0
44.80	296.0
45.90	115.0
46.80	282.0
47.90	227.0
49.00	1325.0
50.00	6289.0
51.00	2153.0
51.90	141.0
54.90	144.0
56.00	477.0
57.00	840.0
59.80	372.0
60.90	1502.0
62.00	2012.0
62.90	1518.0
63.90	181.0
64.90	359.0
67.90	3619.0
68.90	3743.0
70.00	335.0
71.70	232.0
73.00	1706.0
74.00	6435.0
75.00	19840.0
76.00	1739.0
76.80	171.0
77.70	162.0
78.90	1123.0
79.90	266.0
80.80	966.0
81.90	209.0
87.00	1551.0
87.90	1264.0
90.80	193.0
91.90	1167.0
92.90	1694.0
93.90	4817.0
95.00	39952.0
96.00	2943.0
103.80	193.0
105.90	188.0
115.80	153.0
116.80	257.0
117.70	125.0
119.00	187.0
127.80	148.0
129.80	165.0
134.60	119.0
141.00	430.0
142.80	634.0
145.00	131.0
148.00	126.0
170.70	117.0
171.80	463.0
172.90	666.0
173.90	39736.0
174.90	3184.0
175.90	38032.0
176.90	2412.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64