


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081120\
 Data File : VV017910.D
 Acq On : 11 Aug 2020 15:23
 Operator : SY/MD
 Sample : BFB71
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB71

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 13 14:37:38 2020

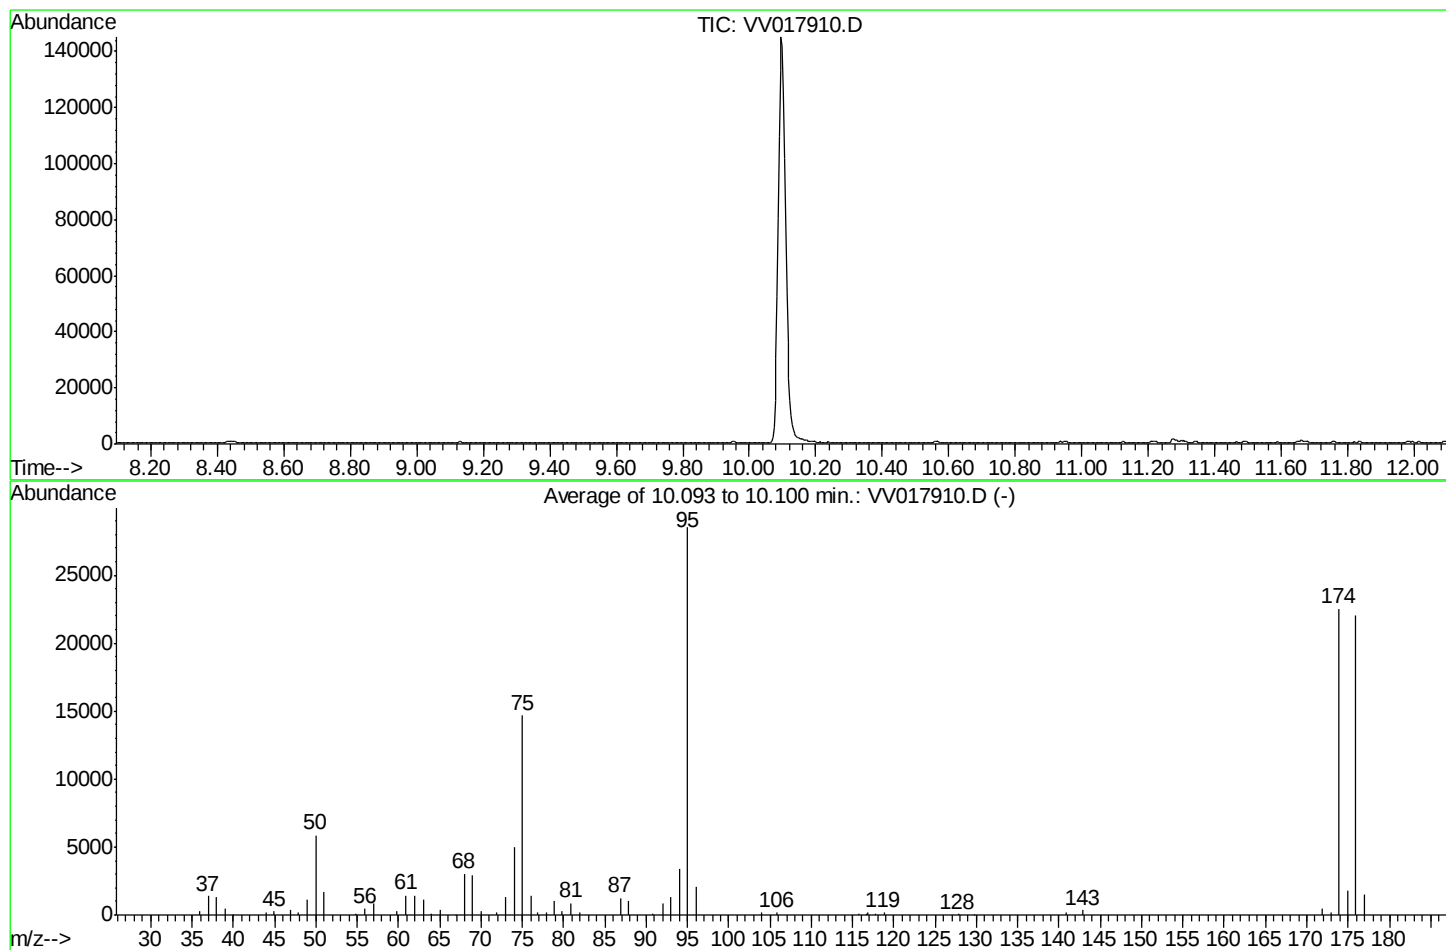

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	5848	PASS
75	95	30	80	51.5	14679	PASS
95	95	100	100	100.0	28517	PASS
96	95	5	9	7.4	2110	PASS
173	174	0.00	2	1.0	222	PASS
174	95	50	120	79.1	22544	PASS
175	174	5	9	7.8	1759	PASS
176	174	95	101	97.7	22016	PASS
177	176	5	9	6.9	1513	PASS

m/z	Abundance
35.90	295.0
37.00	1371.0
38.00	1269.0
38.90	524.0
39.90	183.0
44.00	503.0
44.90	281.0
47.00	364.0
47.80	202.0
49.00	1068.0
50.00	5601.0
51.00	1620.0
54.90	117.0
55.90	379.0
57.00	850.0
59.90	258.0
61.00	1409.0
62.00	1381.0
63.00	1116.0
64.00	161.0
65.00	305.0
66.90	102.0
68.00	2918.0
69.00	2852.0
70.00	280.0
71.90	148.0
73.00	1164.0
74.00	4832.0
75.00	13941.0
76.00	1428.0
77.00	213.0
77.90	162.0
78.80	983.0
79.80	265.0
80.90	840.0
81.90	215.0
86.90	1129.0
87.80	950.0
91.00	109.0
92.00	805.0
92.90	1197.0
94.00	3314.0
95.00	27232.0
96.00	2092.0
103.90	164.0
105.90	164.0
115.80	122.0
116.70	186.0
117.70	101.0
118.80	157.0
140.80	213.0
142.90	376.0
171.90	451.0
172.90	323.0
173.90	20896.0
174.90	1750.0
175.90	20448.0
176.90	1411.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	333.0
37.00	1478.0
38.00	1376.0
38.90	514.0
39.90	186.0
44.00	521.0
45.00	278.0
47.00	373.0
47.80	219.0
49.00	1147.0
50.00	6083.0
51.00	1783.0
54.90	120.0
56.00	437.0
57.00	853.0
59.80	292.0
60.90	1518.0
62.00	1458.0
63.00	1157.0
64.10	145.0
65.00	350.0
68.00	3142.0
69.00	3066.0
70.00	268.0
72.00	172.0
73.00	1328.0
74.00	5145.0
75.00	15180.0
76.00	1501.0
76.90	208.0
77.90	188.0
78.80	1042.0
79.80	287.0
80.90	897.0
81.80	211.0
86.90	1302.0
87.80	1060.0
90.80	128.0
92.00	858.0
92.90	1333.0
94.00	3556.0
95.00	29584.0
96.00	2214.0
103.90	159.0
105.90	151.0
115.80	126.0
116.90	223.0
117.80	110.0
118.90	161.0
127.80	138.0
140.80	237.0
142.90	353.0
171.90	463.0
172.90	343.0
173.90	23320.0
174.90	1825.0
175.90	22752.0
176.90	1574.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	330.0
37.00	1373.0
38.00	1302.0
39.00	503.0
39.90	195.0
44.00	481.0
45.00	278.0
47.00	380.0
47.90	198.0
49.00	1132.0
50.00	5862.0
51.00	1767.0
54.90	111.0
56.00	466.0
57.00	775.0
59.90	287.0
60.90	1434.0
62.00	1433.0
63.00	1108.0
64.10	111.0
65.00	371.0
68.00	3002.0
69.00	2927.0
70.00	242.0
72.00	160.0
73.00	1346.0
74.00	4979.0
75.00	14918.0
76.00	1389.0
76.80	213.0
77.80	166.0
78.80	997.0
79.80	255.0
80.90	925.0
82.00	186.0
86.90	1274.0
87.90	1068.0
90.80	139.0
92.00	826.0
92.90	1320.0
94.00	3438.0
95.00	28736.0
96.00	2024.0
103.90	127.0
105.90	139.0
115.80	103.0
116.90	247.0
118.90	161.0
127.80	145.0
129.70	115.0
140.80	259.0
142.90	339.0
171.80	420.0
173.90	23416.0
174.90	1702.0
175.90	22848.0
176.90	1556.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Scan 2790 (10.061 min): VV017910.D
BFB71

m/z	Abundance
39.90	176.0
43.90	287.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71