

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027277.D
 Acq On : 11 Aug 2022 10:46
 Operator : SY/MD
 Sample : VV0811WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK259

Quant Time: Aug 12 03:41:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 12 03:40:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	336120	50.000	ug/L	# 0.00
28) Chlorobenzene-d5	8.850	117	334202	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	138519	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	108747	47.455	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.900%
7) Chloroethane-d5	1.558	69	87058	51.966	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.940%
11) 1,1-Dichloroethene-d2	2.101	63	149763	35.729	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.460%
21) 2-Butanone-d5	3.870	46	171330	83.994	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.990%
24) Chloroform-d	4.342	84	207522	44.209	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.420%
26) 1,2-Dichloroethane-d4	5.027	65	137841	47.296	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.600%
32) Benzene-d6	5.043	84	407808	50.885	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.760%
36) 1,2-Dichloropropane-d6	6.066	67	144278	50.609	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.220%
41) Toluene-d8	7.313	98	339245	49.661	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.320%
43) trans-1,3-Dichloroprop...	7.619	79	57709	46.441	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.880%
47) 2-Hexanone-d5	8.085	63	108497	79.017	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.020%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	195903	42.167	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.340%
66) 1,2-Dichlorobenzene-d4	11.622	152	125856	52.613	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.220%
Target Compounds						
35) Methylcyclohexane	6.066	83	32519	8.042	ug/L	# 21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027277.D
Acq On : 11 Aug 2022 10:46
Operator : SY/MD
Sample : VV0811WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK259

Quant Time: Aug 12 03:41:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 12 03:40:21 2022
Response via : Initial Calibration

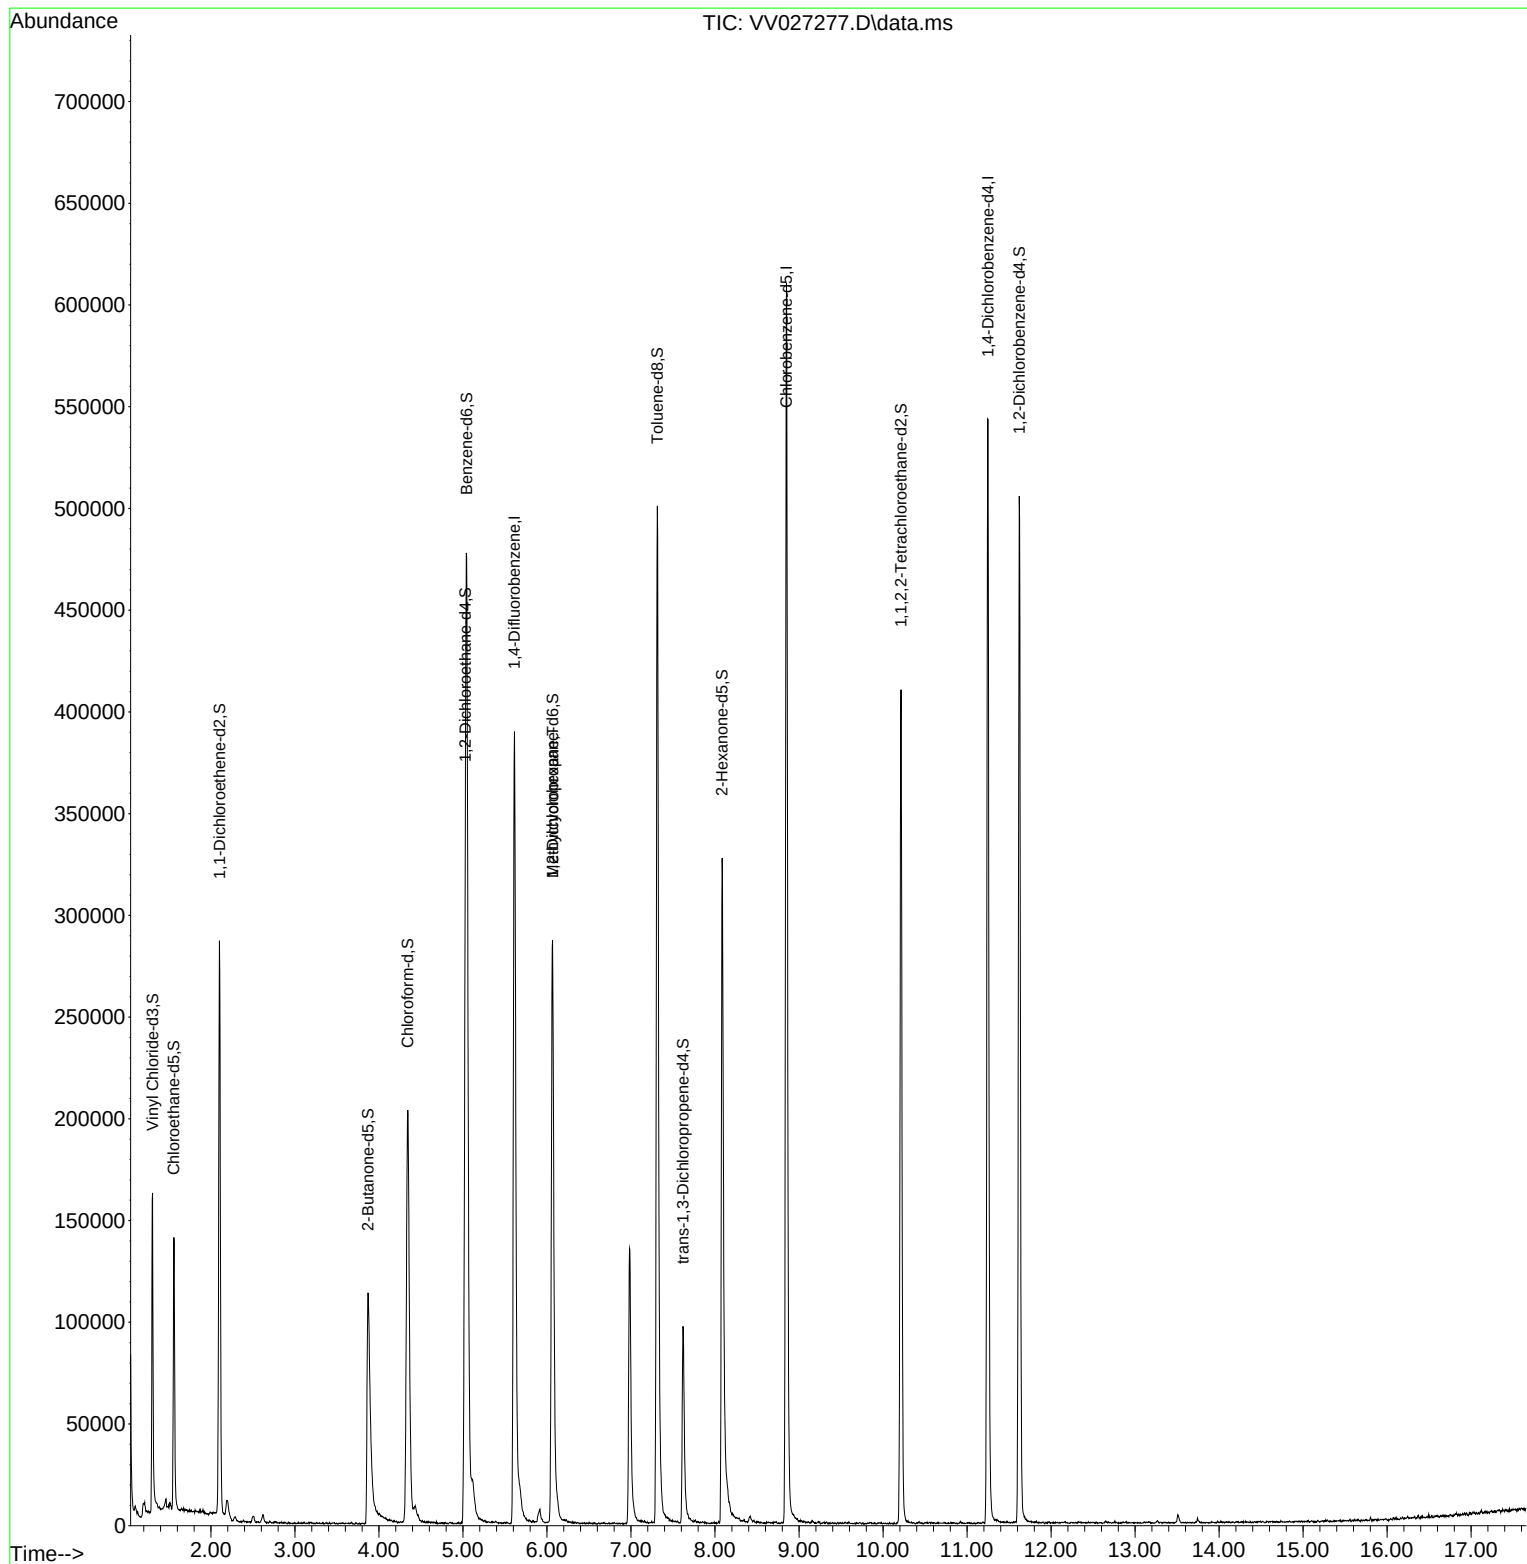

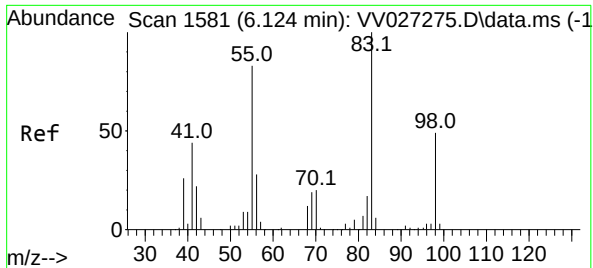

#35
 Methylcyclohexane
 Concen: 8.042 ug/L
 RT: 6.066 min Scan# 11
 Delta R.T. -0.058 min
 Lab File: VV027277.D
 Acq: 11 Aug 2022 10:46

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK259

Tgt Ion:	83	Resp:	32519
Ion	Ratio	Lower	Upper
83	100		
55	0.4	55.5	83.3#
98	0.7	39.0	58.4#

