

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027277.D
 Acq On : 11 Aug 2022 10:46
 Operator : SY/MD
 Sample : VV0811WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	156850	169943	13.80%	1.769%
2	1.558	155	161	182	rVB	134197	160410	13.03%	1.670%
3	2.101	321	330	344	rVB	281167	396180	32.18%	4.124%
4	2.696	513	515	516	rBV2	741	315	0.03%	0.003%
5	2.876	568	571	572	rBV3	540	242	0.02%	0.003%
6	2.921	581	585	588	rBV4	802	633	0.05%	0.007%
7	2.998	606	609	612	rVB3	594	388	0.03%	0.004%
8	3.043	621	623	626	rBV4	595	230	0.02%	0.002%
9	3.166	658	661	664	rBV2	736	578	0.05%	0.006%
10	3.230	679	681	683	rBV2	482	254	0.02%	0.003%
11	3.256	685	689	692	rBV6	653	496	0.04%	0.005%
12	3.291	698	700	703	rVB2	497	242	0.02%	0.003%
13	3.371	720	725	730	rVV5	662	635	0.05%	0.007%
14	3.410	734	737	740	rBV	643	341	0.03%	0.004%
15	3.490	760	762	766	rVB3	577	337	0.03%	0.004%
16	3.526	770	773	775	rBV2	482	260	0.02%	0.003%
17	3.674	816	819	822	rVB2	791	559	0.05%	0.006%
18	3.722	830	834	835	rBV2	688	373	0.03%	0.004%
19	3.760	843	846	847	rBV2	462	267	0.02%	0.003%
20	3.796	854	857	859	rBV2	343	229	0.02%	0.002%
21	3.838	867	870	871	rBV	826	432	0.04%	0.004%
22	3.870	871	880	911	rVV	113177	320549	26.04%	3.337%
23	4.342	1013	1027	1047	rBV	201132	498523	40.49%	5.190%
24	4.619	1111	1113	1117	rBV3	696	391	0.03%	0.004%
25	4.683	1132	1133	1136	rVB	1233	369	0.03%	0.004%
26	4.699	1136	1138	1141	rBV2	605	360	0.03%	0.004%
27	4.812	1171	1173	1177	rVB3	488	254	0.02%	0.003%
28	4.844	1177	1183	1189	rBV6	851	1258	0.10%	0.013%
29	4.982	1221	1226	1228	rBV4	1134	788	0.06%	0.008%
30	5.040	1228	1244	1263	rBV2	476868	1231097	100.00%	12.816%
31	5.439	1363	1368	1371	rBV6	595	597	0.05%	0.006%
32	5.612	1409	1422	1464	rVV	389350	833848	67.73%	8.680%
33	5.915	1505	1516	1523	rBV	6141	12068	0.98%	0.126%
34	6.066	1551	1563	1596	rBV	285167	603504	49.02%	6.282%
35	6.317	1639	1641	1643	rBV2	630	257	0.02%	0.003%
36	6.468	1686	1688	1690	rBV4	465	217	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027277.D
 Acq On : 11 Aug 2022 10:46
 Operator : SY/MD
 Sample : VV0811WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.500	1695	1698	1700	rBV2	663	322	0.03%	0.003%
38	6.551	1713	1714	1716	rBV2	612	316	0.03%	0.003%
39	6.619	1730	1735	1736	rBV2	476	367	0.03%	0.004%
40	6.648	1739	1744	1746	rBV4	622	536	0.04%	0.006%
41	6.706	1760	1762	1767	rBV3	392	289	0.02%	0.003%
42	6.757	1776	1778	1781	rBV2	312	200	0.02%	0.002%
43	6.780	1781	1785	1787	rVV3	458	352	0.03%	0.004%
44	6.831	1799	1801	1803	rVB	548	195	0.02%	0.002%
45	6.918	1825	1828	1831	rBV	475	391	0.03%	0.004%
46	6.940	1831	1835	1837	rVV2	547	370	0.03%	0.004%
47	6.982	1837	1848	1877	rBV	135467	265860	21.60%	2.768%
48	7.313	1939	1951	1983	rBV	499846	916299	74.43%	9.539%
49	7.619	2036	2046	2063	rBV	96648	175790	14.28%	1.830%
50	7.751	2086	2087	2089	rBV2	827	343	0.03%	0.004%
51	7.828	2108	2111	2113	rBV3	655	426	0.03%	0.004%
52	7.960	2151	2152	2156	rVB4	394	242	0.02%	0.003%
53	8.043	2176	2178	2180	rVB3	908	356	0.03%	0.004%
54	8.085	2181	2191	2224	rBV	326862	639427	51.94%	6.656%
55	8.500	2318	2320	2322	rBV2	634	288	0.02%	0.003%
56	8.612	2353	2355	2356	rBV	838	311	0.03%	0.003%
57	8.709	2381	2385	2387	rBV3	860	757	0.06%	0.008%
58	8.779	2405	2407	2409	rBV2	392	212	0.02%	0.002%
59	8.796	2409	2412	2415	rBV3	696	433	0.04%	0.005%
60	8.850	2417	2429	2452	rBV	609324	1019447	82.81%	10.612%
61	9.140	2517	2519	2520	rBV	567	197	0.02%	0.002%
62	9.152	2520	2523	2524	rBV2	1045	467	0.04%	0.005%
63	9.246	2549	2552	2556	rVB4	1190	813	0.07%	0.008%
64	9.268	2556	2559	2561	rBV3	450	347	0.03%	0.004%
65	9.355	2584	2586	2589	rBV2	546	268	0.02%	0.003%
66	9.390	2594	2597	2598	rBV2	408	242	0.02%	0.003%
67	9.548	2645	2646	2650	rVB	649	383	0.03%	0.004%
68	9.667	2679	2683	2685	rVB2	524	421	0.03%	0.004%
69	9.683	2685	2688	2689	rBV	739	408	0.03%	0.004%
70	9.760	2708	2712	2715	rVB2	773	620	0.05%	0.006%
71	9.789	2719	2721	2723	rBV3	430	307	0.02%	0.003%
72	9.834	2733	2735	2737	rBV2	467	268	0.02%	0.003%
73	9.898	2751	2755	2757	rVB4	620	451	0.04%	0.005%
74	9.911	2757	2759	2763	rVB2	423	224	0.02%	0.002%
75	9.940	2763	2768	2770	rBV2	578	523	0.04%	0.005%
76	9.979	2778	2780	2784	rVB3	752	383	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027277.D
 Acq On : 11 Aug 2022 10:46
 Operator : SY/MD
 Sample : VV0811WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.004	2784	2788	2791	rBV2	438	370	0.03%	0.004%
78	10.075	2808	2810	2814	rBV4	647	393	0.03%	0.004%
79	10.120	2821	2824	2826	rVB2	620	271	0.02%	0.003%
80	10.133	2826	2828	2833	rBV3	753	483	0.04%	0.005%
81	10.213	2842	2853	2873	rVB	409292	647048	52.56%	6.736%
82	10.339	2890	2892	2896	rVB3	565	296	0.02%	0.003%
83	10.484	2935	2937	2939	rBV	369	231	0.02%	0.002%
84	10.496	2939	2941	2944	rVV3	480	373	0.03%	0.004%
85	10.577	2963	2966	2970	rBV4	688	598	0.05%	0.006%
86	10.808	3033	3038	3039	rBV3	764	491	0.04%	0.005%
87	10.898	3063	3066	3069	rBV3	380	334	0.03%	0.003%
88	11.082	3120	3123	3126	rBV2	517	389	0.03%	0.004%
89	11.117	3130	3134	3135	rBV2	387	302	0.02%	0.003%
90	11.246	3163	3174	3199	rBV	542929	866176	70.36%	9.017%
91	11.622	3280	3291	3310	rBV	504158	811236	65.90%	8.445%
92	11.937	3385	3389	3391	rBV3	704	550	0.04%	0.006%
93	11.963	3395	3397	3400	rBV4	766	480	0.04%	0.005%
94	12.033	3417	3419	3421	rVB3	593	202	0.02%	0.002%
95	12.638	3604	3607	3608	rBV2	552	264	0.02%	0.003%
96	13.033	3729	3730	3734	rBV2	418	264	0.02%	0.003%
97	13.464	3862	3864	3866	rBV	431	230	0.02%	0.002%
98	13.509	3873	3878	3892	rVB3	4087	6460	0.52%	0.067%
99	13.744	3948	3951	3955	rBV6	1787	1104	0.09%	0.011%
100	14.371	4145	4146	4151	rVB3	718	405	0.03%	0.004%




Sum of corrected areas: 9606225

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027277.D
Acq On : 11 Aug 2022 10:46
Operator : SY/MD
Sample : VV0811WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

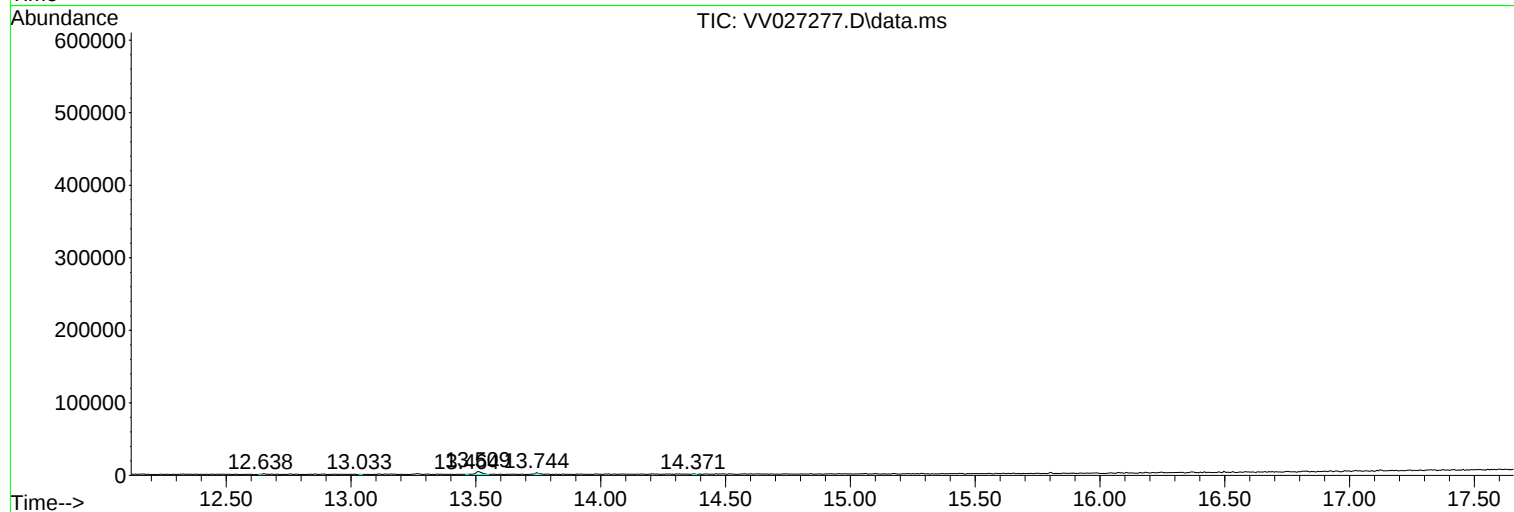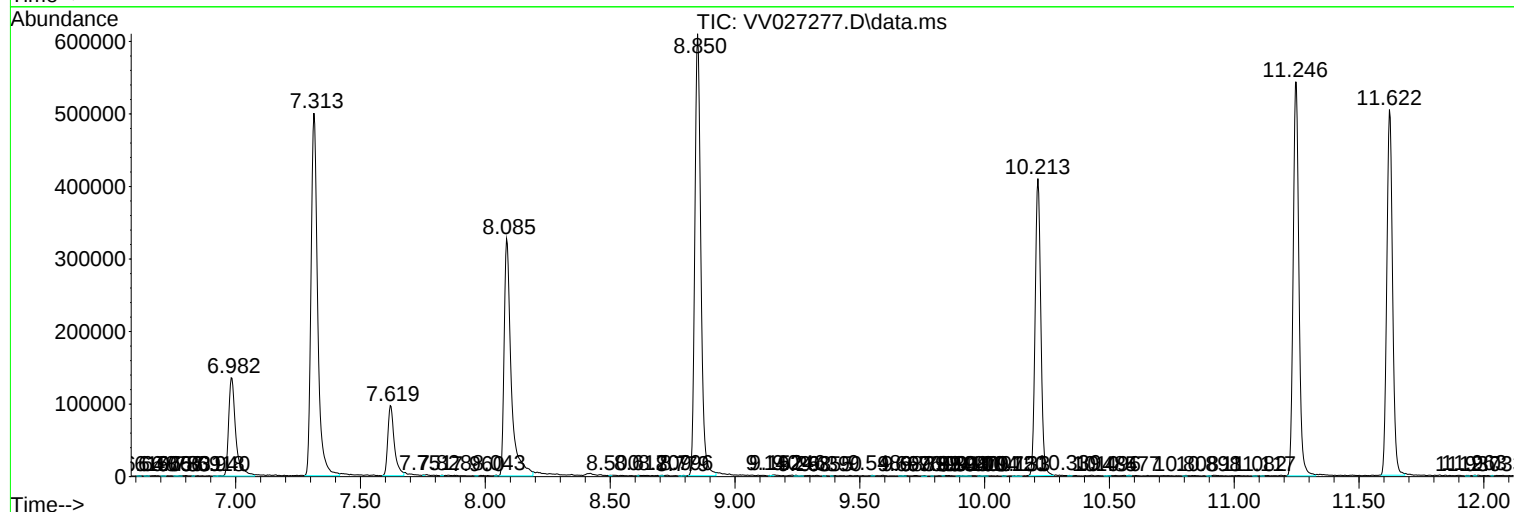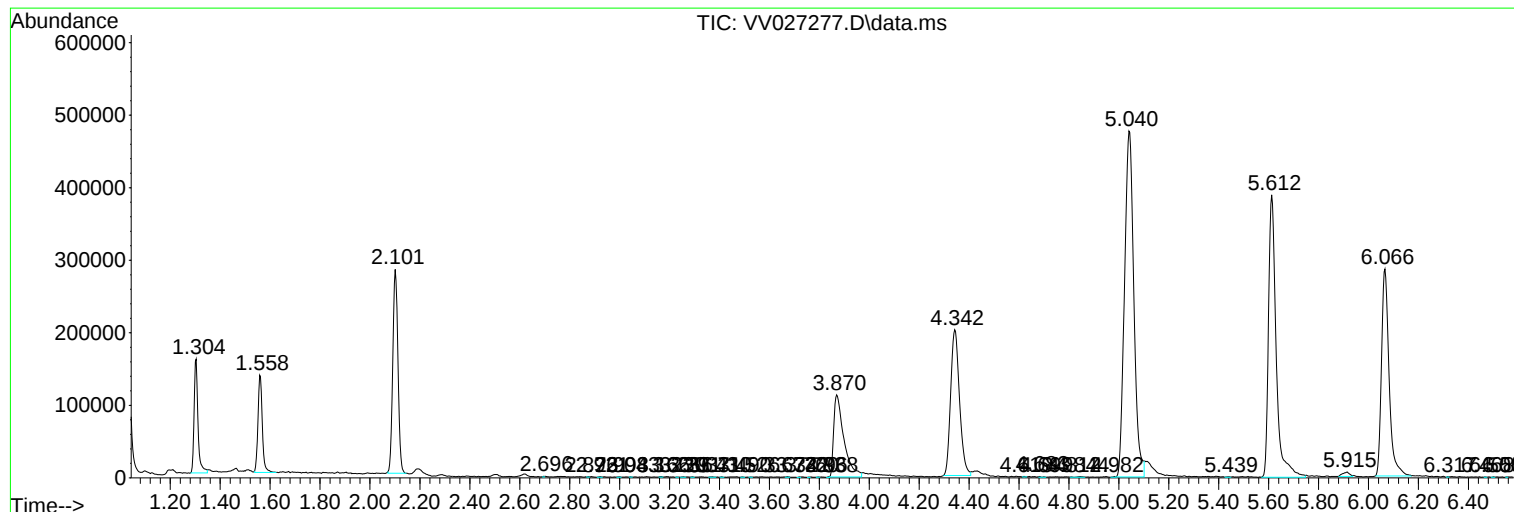

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027277.D
Acq On : 11 Aug 2022 10:46
Operator : SY/MD
Sample : VV0811WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027277.D
Acq On : 11 Aug 2022 10:46
Operator : SY/MD
Sample : VV0811WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------