

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027278.D
 Acq On : 11 Aug 2022 11:19
 Operator : SY/MD
 Sample : N4144-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rBV	213311	237926	14.64%	1.990%
2	1.561	155	162	178	rVB	176483	213910	13.16%	1.790%
3	2.101	321	330	341	rBV	367642	512576	31.54%	4.288%
4	2.677	507	509	512	rBV2	857	380	0.02%	0.003%
5	2.696	512	515	517	rBV2	569	358	0.02%	0.003%
6	2.728	523	525	526	rBV3	426	236	0.01%	0.002%
7	2.764	527	536	547	rVB3	3442	6920	0.43%	0.058%
8	2.886	570	574	577	rBV3	688	523	0.03%	0.004%
9	2.940	587	591	595	rBV4	854	780	0.05%	0.007%
10	3.066	625	630	633	rBV3	1032	975	0.06%	0.008%
11	3.114	642	645	649	rBV3	770	537	0.03%	0.004%
12	3.185	654	667	684	rBV2	24737	54094	3.33%	0.453%
13	3.346	715	717	719	rBV2	388	251	0.02%	0.002%
14	3.397	726	733	734	rBV4	757	702	0.04%	0.006%
15	3.484	758	760	762	rVB	559	240	0.01%	0.002%
16	3.513	764	769	773	rBV5	1194	1324	0.08%	0.011%
17	3.651	811	812	814	rBV	595	219	0.01%	0.002%
18	3.683	820	822	825	rVB3	592	225	0.01%	0.002%
19	3.744	839	841	845	rVB2	665	379	0.02%	0.003%
20	3.773	848	850	853	rVB2	458	218	0.01%	0.002%
21	3.818	860	864	868	rVB3	768	560	0.03%	0.005%
22	3.866	868	879	908	rBV	133573	405362	24.94%	3.391%
23	4.339	1012	1026	1048	rBV	260020	656490	40.40%	5.492%
24	4.702	1137	1139	1145	rVB4	1418	808	0.05%	0.007%
25	4.764	1156	1158	1160	rBV	397	235	0.01%	0.002%
26	4.973	1221	1223	1227	rVB4	613	379	0.02%	0.003%
27	5.037	1227	1243	1264	rBV2	622019	1625098	100.00%	13.596%
28	5.381	1348	1350	1354	rBV3	487	267	0.02%	0.002%
29	5.407	1354	1358	1359	rBV3	577	442	0.03%	0.004%
30	5.439	1364	1368	1372	rVB5	773	684	0.04%	0.006%
31	5.529	1392	1396	1399	rBV4	661	517	0.03%	0.004%
32	5.555	1399	1404	1405	rBV4	935	702	0.04%	0.006%
33	5.609	1409	1421	1461	rBV	406459	883553	54.37%	7.392%
34	5.908	1506	1514	1524	rBV8	6685	14239	0.88%	0.119%
35	6.001	1542	1543	1546	rBV3	493	271	0.02%	0.002%
36	6.063	1546	1562	1590	rBV	365543	790170	48.62%	6.611%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027278.D
 Acq On : 11 Aug 2022 11:19
 Operator : SY/MD
 Sample : N4144-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.490	1689	1695	1697	rBV6	714	790	0.05%	0.007%
38	6.641	1740	1742	1744	rVB2	661	275	0.02%	0.002%
39	6.657	1744	1747	1748	rBV	567	389	0.02%	0.003%
40	6.802	1790	1792	1794	rBV3	701	431	0.03%	0.004%
41	6.934	1828	1833	1836	rBV4	1038	993	0.06%	0.008%
42	6.982	1836	1848	1872	rBV	155866	298697	18.38%	2.499%
43	7.214	1918	1920	1923	rVB3	1000	445	0.03%	0.004%
44	7.310	1938	1950	1974	rBV	661740	1217909	74.94%	10.189%
45	7.619	2036	2046	2070	rBV	113156	209924	12.92%	1.756%
46	7.982	2149	2159	2165	rBV8	4629	7276	0.45%	0.061%
47	8.043	2176	2178	2179	rBV2	518	257	0.02%	0.002%
48	8.085	2180	2191	2220	rBV	434445	829173	51.02%	6.937%
49	8.477	2311	2313	2315	rBV2	752	300	0.02%	0.003%
50	8.497	2317	2319	2321	rBV2	643	252	0.02%	0.002%
51	8.564	2337	2340	2341	rBV2	802	434	0.03%	0.004%
52	8.667	2370	2372	2377	rVB4	734	467	0.03%	0.004%
53	8.715	2384	2387	2393	rVB4	1017	834	0.05%	0.007%
54	8.847	2418	2428	2458	rBV	656011	1098200	67.58%	9.188%
55	9.149	2516	2522	2527	rBV4	2026	2296	0.14%	0.019%
56	9.226	2545	2546	2548	rBV2	471	219	0.01%	0.002%
57	9.284	2561	2564	2570	rBV5	385	399	0.02%	0.003%
58	9.326	2575	2577	2580	rVB3	1039	391	0.02%	0.003%
59	9.381	2590	2594	2595	rBV	567	416	0.03%	0.003%
60	9.487	2624	2627	2631	rBV3	346	302	0.02%	0.003%
61	9.506	2631	2633	2634	rBV	993	409	0.03%	0.003%
62	9.696	2690	2692	2695	rVB4	754	382	0.02%	0.003%
63	9.722	2695	2700	2701	rBV3	564	379	0.02%	0.003%
64	9.731	2701	2703	2705	rBV3	548	293	0.02%	0.002%
65	9.802	2721	2725	2729	rVB4	501	414	0.03%	0.003%
66	9.824	2729	2732	2733	rBV2	680	268	0.02%	0.002%
67	9.847	2737	2739	2743	rVB3	538	290	0.02%	0.002%
68	9.882	2748	2750	2753	rVB2	469	275	0.02%	0.002%
69	9.908	2755	2758	2760	rBV3	406	312	0.02%	0.003%
70	9.934	2760	2766	2769	rBV7	1706	1628	0.10%	0.014%
71	10.017	2788	2792	2794	rBV3	530	411	0.03%	0.003%
72	10.101	2816	2818	2823	rVB3	413	321	0.02%	0.003%
73	10.140	2825	2830	2834	rVB3	567	657	0.04%	0.005%
74	10.214	2839	2853	2877	rBV	534505	847128	52.13%	7.087%
75	10.468	2927	2932	2936	rBV3	871	847	0.05%	0.007%
76	10.586	2966	2969	2973	rVB3	1189	713	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027278.D
 Acq On : 11 Aug 2022 11:19
 Operator : SY/MD
 Sample : N4144-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.818	3039	3041	3045	rVB	537	395	0.02%	0.003%
78	10.850	3049	3051	3053	rVV3	824	462	0.03%	0.004%
79	10.886	3060	3062	3067	rBV4	960	554	0.03%	0.005%
80	10.918	3067	3072	3075	rBV6	1522	1181	0.07%	0.010%
81	10.982	3087	3092	3095	rBV3	595	585	0.04%	0.005%
82	11.188	3152	3156	3161	rBV4	1266	1318	0.08%	0.011%
83	11.246	3163	3174	3197	rBV	578884	920354	56.63%	7.700%
84	11.541	3257	3266	3275	rBV6	6710	14197	0.87%	0.119%
85	11.622	3280	3291	3312	rVV	675267	1065346	65.56%	8.913%
86	11.966	3396	3398	3400	rBV2	559	253	0.02%	0.002%
87	12.339	3512	3514	3518	rBV3	843	534	0.03%	0.004%
88	12.615	3598	3600	3604	rVB3	700	317	0.02%	0.003%
89	12.641	3604	3608	3619	rVB8	1542	2785	0.17%	0.023%
90	12.750	3639	3642	3645	rBV	980	555	0.03%	0.005%
91	12.966	3706	3709	3710	rBV2	472	296	0.02%	0.002%
92	13.258	3796	3800	3804	rBV6	1154	1315	0.08%	0.011%
93	13.326	3816	3821	3825	rBV5	771	708	0.04%	0.006%
94	13.438	3854	3856	3859	rBV2	774	416	0.03%	0.003%
95	13.477	3866	3868	3871	rBV3	482	334	0.02%	0.003%
96	13.651	3919	3922	3925	rBV3	741	477	0.03%	0.004%
97	13.718	3940	3943	3946	rBV4	1088	687	0.04%	0.006%
98	13.905	3999	4001	4005	rVB4	685	393	0.02%	0.003%
99	14.352	4138	4140	4145	rBV5	794	827	0.05%	0.007%
100	14.930	4318	4320	4323	rBV3	658	443	0.03%	0.004%




Sum of corrected areas: 11953078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027278.D
Acq On : 11 Aug 2022 11:19
Operator : SY/MD
Sample : N4144-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

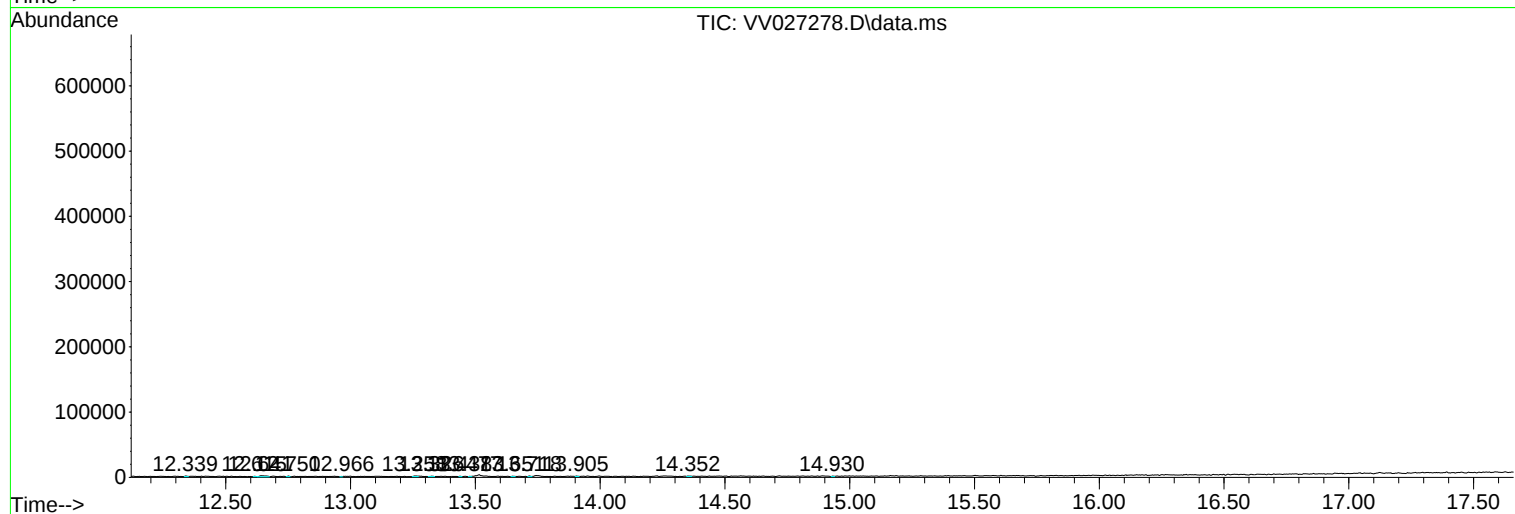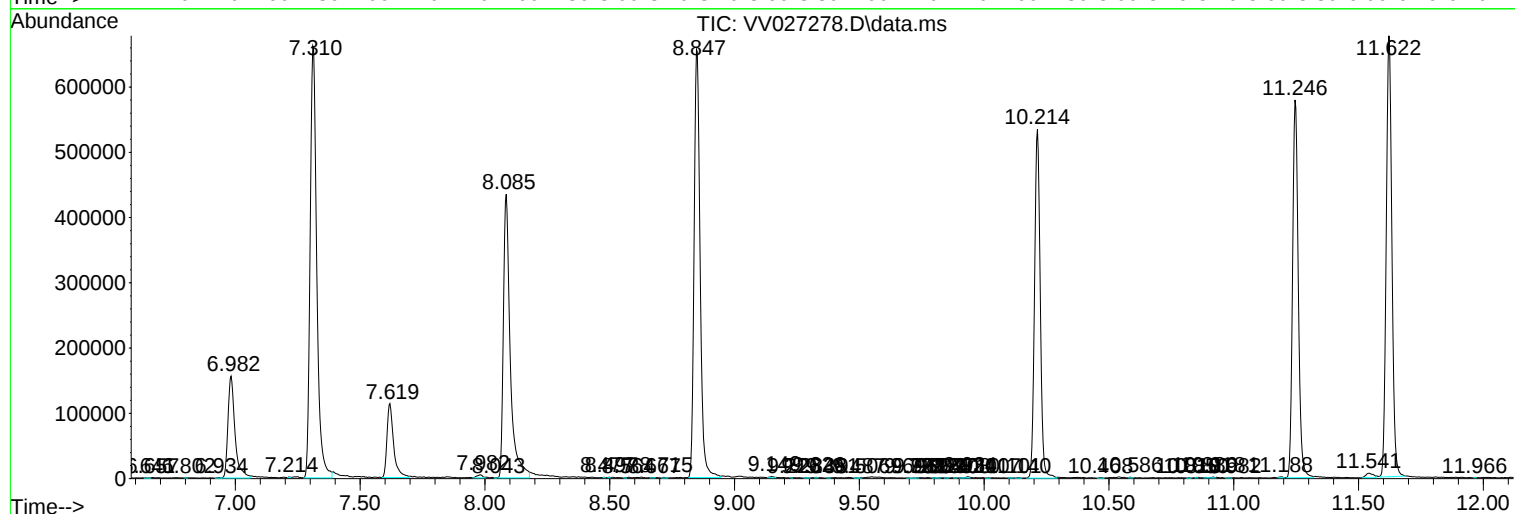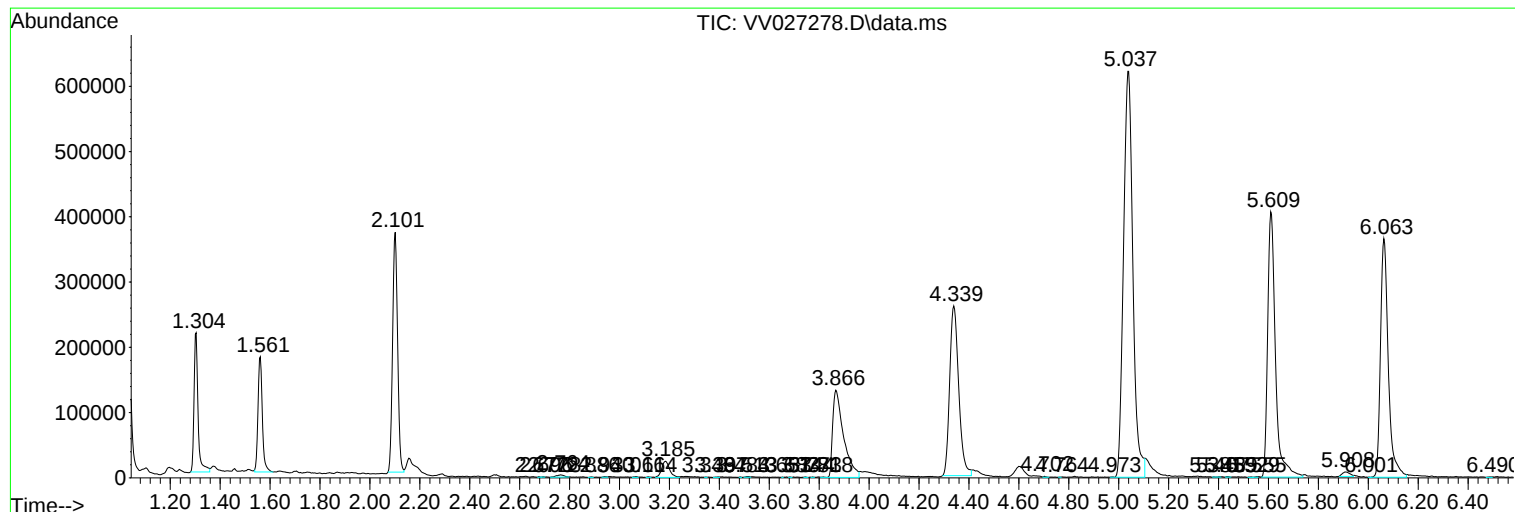

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027278.D
Acq On : 11 Aug 2022 11:19
Operator : SY/MD
Sample : N4144-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027278.D
Acq On : 11 Aug 2022 11:19
Operator : SY/MD
Sample : N4144-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc