

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027279.D
 Acq On : 11 Aug 2022 11:44
 Operator : SY/MD
 Sample : N4144-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY153

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rBV	171512	183627	1.09%	0.518%
2	1.561	155	162	176	rVB	145781	172589	1.02%	0.487%
3	2.101	321	330	342	rBV2	291989	419102	2.48%	1.181%
4	2.581	478	479	485	rBV4	689	388	0.00%	0.001%
5	2.703	515	517	519	rBV3	484	198	0.00%	0.001%
6	2.751	519	532	551	rBV	1719708	2930614	17.32%	8.262%
7	3.166	658	661	662	rBV2	627	301	0.00%	0.001%
8	3.252	684	688	690	rVB6	832	564	0.00%	0.002%
9	3.330	709	712	715	rBV2	618	418	0.00%	0.001%
10	3.413	734	738	740	rBV3	357	286	0.00%	0.001%
11	3.442	744	747	751	rVB3	654	540	0.00%	0.002%
12	3.490	759	762	765	rBV4	602	524	0.00%	0.001%
13	3.513	767	769	770	rVV	532	207	0.00%	0.001%
14	3.523	770	772	775	rVB3	884	497	0.00%	0.001%
15	3.535	775	776	777	rBV	475	133	0.00%	0.000%
16	3.555	780	782	785	rVB3	1030	488	0.00%	0.001%
17	3.597	792	795	798	rBV4	657	542	0.00%	0.002%
18	3.632	802	806	810	rVB4	965	801	0.00%	0.002%
19	3.648	810	811	812	rBV	317	98	0.00%	0.000%
20	3.661	814	815	817	rBV2	348	140	0.00%	0.000%
21	3.696	823	826	827	rVB2	415	187	0.00%	0.001%
22	3.706	827	829	831	rBV3	206	103	0.00%	0.000%
23	3.767	846	848	849	rBV	465	178	0.00%	0.001%
24	3.783	852	853	857	rVB3	568	324	0.00%	0.001%
25	3.902	870	890	910	rBV2	2239672	5529663	32.69%	15.589%
26	4.342	1013	1027	1048	rBV	232317	574845	3.40%	1.621%
27	4.732	1146	1148	1149	rBV	568	199	0.00%	0.001%
28	4.786	1163	1165	1168	rVB3	692	353	0.00%	0.001%
29	4.883	1192	1195	1196	rBV	651	430	0.00%	0.001%
30	5.040	1227	1244	1262	rBV2	544781	1413433	8.36%	3.985%
31	5.458	1372	1374	1376	rBV2	629	398	0.00%	0.001%
32	5.497	1382	1386	1391	rBV4	898	1000	0.01%	0.003%
33	5.523	1391	1394	1397	rBV4	944	589	0.00%	0.002%
34	5.613	1410	1422	1459	rBV	369859	792477	4.68%	2.234%
35	5.908	1498	1514	1550	rBV	8542622	16917020	100.00%	47.691%
36	6.066	1554	1563	1599	rVB	332013	721704	4.27%	2.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027279.D
 Acq On : 11 Aug 2022 11:44
 Operator : SY/MD
 Sample : N4144-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY153

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.879	1814	1816	1820	rBV3	489	331	0.00%	0.001%
38	6.928	1829	1831	1833	rBV2	671	359	0.00%	0.001%
39	6.982	1839	1848	1872	rBV	134647	260295	1.54%	0.734%
40	7.313	1939	1951	1985	rBV	561965	1012885	5.99%	2.855%
41	7.619	2037	2046	2067	rBV	98488	180447	1.07%	0.509%
42	8.085	2181	2191	2227	rBV	433062	839032	4.96%	2.365%
43	8.442	2299	2302	2306	rBV5	1110	981	0.01%	0.003%
44	8.764	2400	2402	2404	rBV3	574	279	0.00%	0.001%
45	8.850	2416	2429	2452	rBV	590697	985342	5.82%	2.778%
46	9.220	2541	2544	2548	rVV2	1484	1060	0.01%	0.003%
47	9.239	2548	2550	2556	rVB7	1596	1075	0.01%	0.003%
48	9.281	2561	2563	2564	rBV	343	110	0.00%	0.000%
49	9.342	2581	2582	2584	rBV2	508	237	0.00%	0.001%
50	9.387	2592	2596	2597	rBV3	550	294	0.00%	0.001%
51	9.429	2607	2609	2613	rBV3	557	413	0.00%	0.001%
52	9.545	2642	2645	2646	rBV2	1356	629	0.00%	0.002%
53	9.554	2646	2648	2654	rVB3	988	808	0.00%	0.002%
54	9.619	2666	2668	2670	rBV	343	179	0.00%	0.001%
55	9.673	2682	2685	2687	rBV2	483	235	0.00%	0.001%
56	9.834	2734	2735	2738	rVB2	697	224	0.00%	0.001%
57	9.876	2744	2748	2751	rBV3	350	254	0.00%	0.001%
58	9.940	2766	2768	2770	rBV2	558	242	0.00%	0.001%
59	9.953	2770	2772	2775	rVV4	609	351	0.00%	0.001%
60	10.046	2799	2801	2805	rBV4	593	426	0.00%	0.001%
61	10.140	2828	2830	2832	rBV4	481	172	0.00%	0.000%
62	10.214	2841	2853	2874	rBV	514344	796949	4.71%	2.247%
63	10.378	2902	2904	2908	rBV3	828	522	0.00%	0.001%
64	10.500	2938	2942	2944	rBV2	624	465	0.00%	0.001%
65	10.545	2954	2956	2957	rBV2	511	207	0.00%	0.001%
66	10.625	2977	2981	2983	rBV2	523	440	0.00%	0.001%
67	10.641	2983	2986	2989	rVV3	621	457	0.00%	0.001%
68	10.667	2993	2994	2996	rVB2	499	139	0.00%	0.000%
69	10.693	2999	3002	3005	rBV2	389	352	0.00%	0.001%
70	10.735	3012	3015	3016	rBV2	508	304	0.00%	0.001%
71	10.799	3032	3035	3038	rBV4	546	432	0.00%	0.001%
72	10.950	3081	3082	3084	rBV2	430	222	0.00%	0.001%
73	10.995	3094	3096	3100	rVB3	891	502	0.00%	0.001%
74	11.072	3118	3120	3121	rBV2	424	154	0.00%	0.000%
75	11.104	3126	3130	3133	rBV4	759	692	0.00%	0.002%
76	11.165	3145	3149	3152	rBV5	681	508	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027279.D
 Acq On : 11 Aug 2022 11:44
 Operator : SY/MD
 Sample : N4144-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY153

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	11.246	3163	3174	3195	rBV	503255	794773	4.70%	2.241%
78	11.545	3258	3267	3270	rBV6	3120	4666	0.03%	0.013%
79	11.622	3280	3291	3312	rBV	582593	910732	5.38%	2.567%
80	11.972	3398	3400	3403	rBV3	1101	493	0.00%	0.001%
81	12.033	3417	3419	3420	rBV	541	211	0.00%	0.001%
82	12.107	3440	3442	3445	rBV3	779	337	0.00%	0.001%
83	12.410	3532	3536	3537	rBV2	558	447	0.00%	0.001%
84	12.487	3558	3560	3561	rBV	725	305	0.00%	0.001%
85	12.590	3590	3592	3594	rBV3	419	149	0.00%	0.000%
86	12.757	3640	3644	3646	rBV3	640	494	0.00%	0.001%
87	12.783	3649	3652	3655	rBV3	730	442	0.00%	0.001%
88	12.821	3662	3664	3666	rBV2	698	308	0.00%	0.001%
89	13.037	3729	3731	3733	rBV	475	231	0.00%	0.001%
90	13.123	3756	3758	3762	rVB2	674	430	0.00%	0.001%
91	13.268	3801	3803	3805	rBV	561	322	0.00%	0.001%
92	13.410	3842	3847	3849	rBV2	607	520	0.00%	0.001%
93	13.487	3869	3871	3873	rVB	761	265	0.00%	0.001%
94	13.593	3900	3904	3908	rBV6	698	736	0.00%	0.002%
95	13.686	3931	3933	3934	rBV	560	226	0.00%	0.001%
96	13.754	3952	3954	3958	rVB3	1242	584	0.00%	0.002%
97	13.905	3998	4001	4004	rBV3	887	588	0.00%	0.002%
98	14.082	4054	4056	4059	rBV2	603	393	0.00%	0.001%
99	14.204	4091	4094	4097	rBV3	642	469	0.00%	0.001%
100	14.230	4100	4102	4105	rVV3	658	377	0.00%	0.001%




Sum of corrected areas: 35472463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027279.D
Acq On : 11 Aug 2022 11:44
Operator : SY/MD
Sample : N4144-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

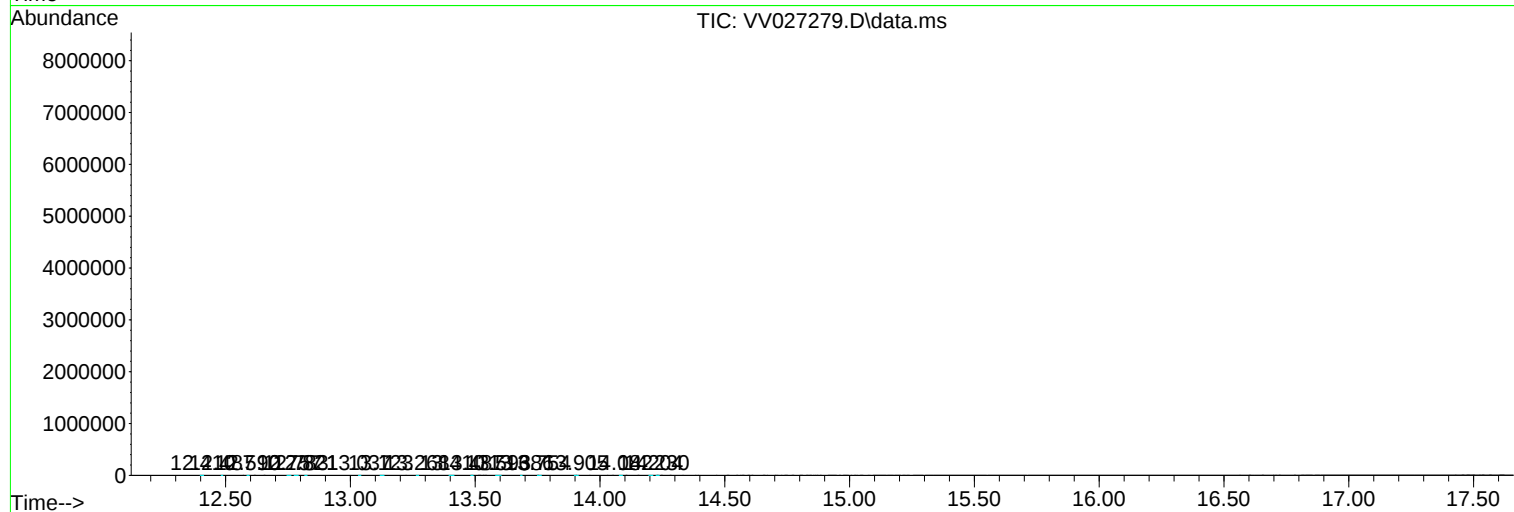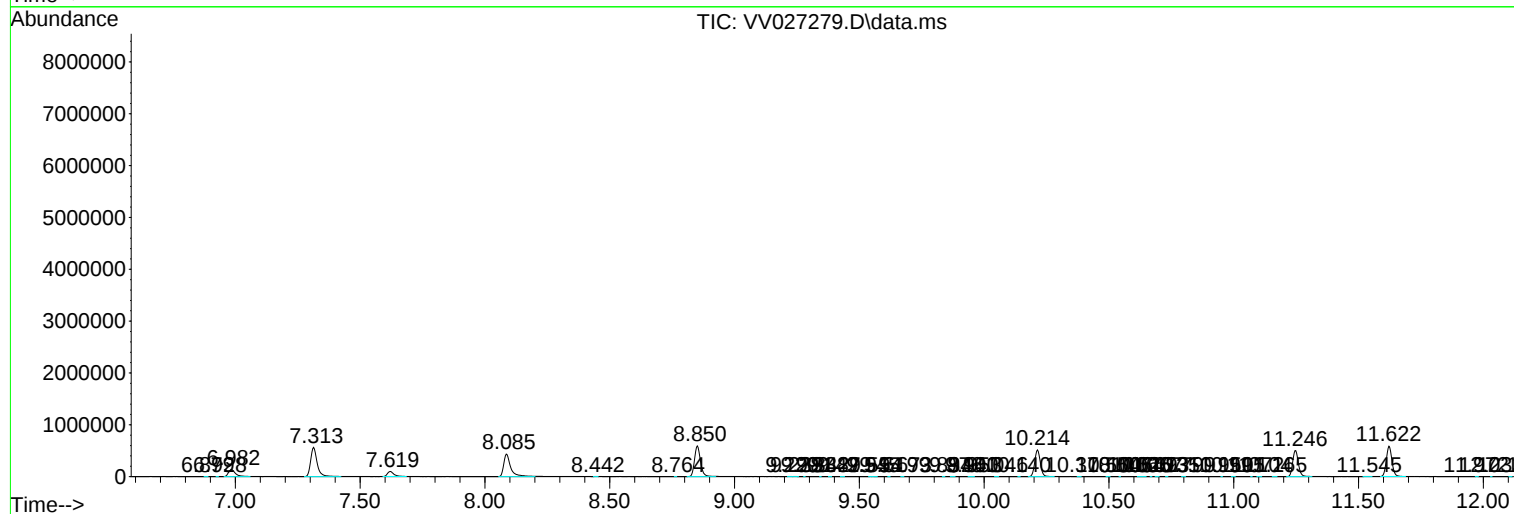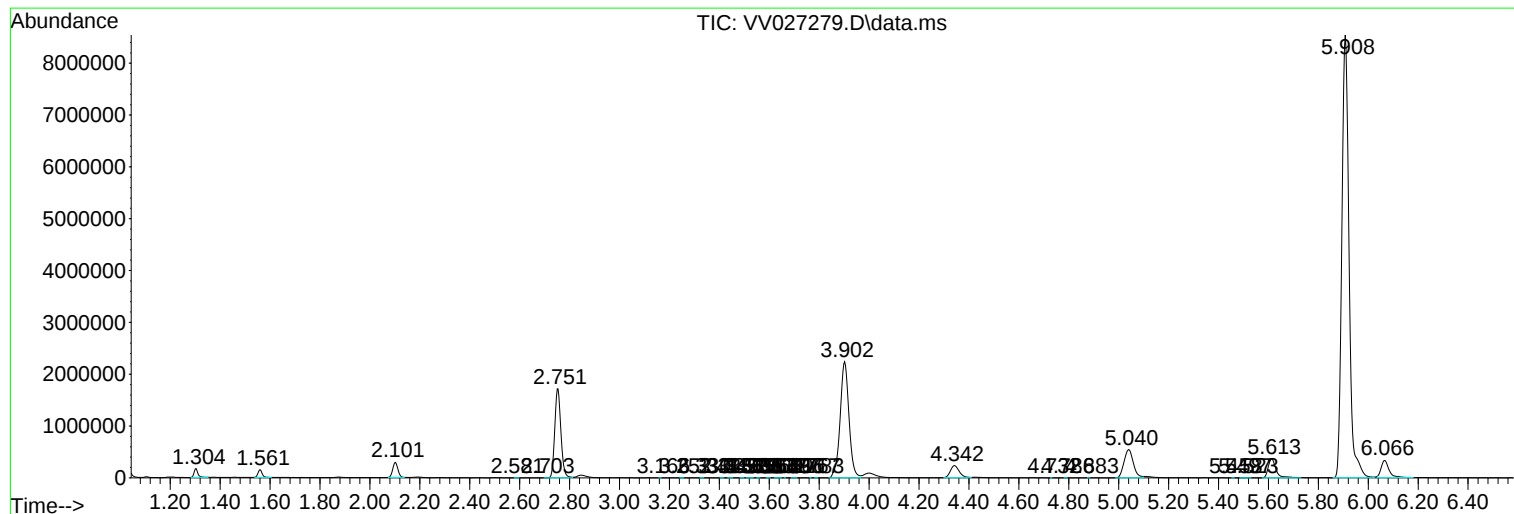

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027279.D
Acq On : 11 Aug 2022 11:44
Operator : SY/MD
Sample : N4144-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027279.D
Acq On : 11 Aug 2022 11:44
Operator : SY/MD
Sample : N4144-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc