

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027280.D
 Acq On : 11 Aug 2022 12:09
 Operator : SY/MD
 Sample : N4144-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027280.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	90	rBV	129000	131230	1.11%	0.468%
2	1.561	155	162	179	rVB	113897	138218	1.17%	0.493%
3	2.101	321	330	344	rBV2	214056	309109	2.61%	1.102%
4	2.455	438	440	442	rBV3	833	340	0.00%	0.001%
5	2.677	507	509	510	rBV2	910	305	0.00%	0.001%
6	2.751	518	532	549	rBV	7065272	11830218	100.00%	42.192%
7	3.243	683	685	688	rVB3	902	324	0.00%	0.001%
8	3.384	727	729	730	rBV2	829	381	0.00%	0.001%
9	3.429	741	743	744	rBV	618	300	0.00%	0.001%
10	3.494	761	763	766	rBV2	953	613	0.01%	0.002%
11	3.535	774	776	777	rBV	563	184	0.00%	0.001%
12	3.596	793	795	798	rBV2	505	359	0.00%	0.001%
13	3.619	798	802	804	rVB4	947	636	0.01%	0.002%
14	3.715	830	832	834	rBV2	445	237	0.00%	0.001%
15	3.767	846	848	852	rBV3	769	414	0.00%	0.001%
16	3.821	863	865	867	rVB2	722	320	0.00%	0.001%
17	3.902	870	890	909	rBV	2539962	6217045	52.55%	22.173%
18	4.342	1014	1027	1046	rBV	193825	474731	4.01%	1.693%
19	4.847	1182	1184	1186	rBV	377	223	0.00%	0.001%
20	4.876	1191	1193	1195	rBV	673	444	0.00%	0.002%
21	4.899	1197	1200	1201	rBV2	519	264	0.00%	0.001%
22	4.960	1218	1219	1222	rBB	669	265	0.00%	0.001%
23	5.040	1228	1244	1285	rVV2	428089	1170066	9.89%	4.173%
24	5.346	1337	1339	1341	rVB2	1436	537	0.00%	0.002%
25	5.497	1383	1386	1390	rVB2	908	705	0.01%	0.003%
26	5.519	1390	1393	1396	rBV2	758	589	0.00%	0.002%
27	5.612	1410	1422	1457	rBV	306401	654610	5.53%	2.335%
28	5.908	1501	1514	1544	rBV	693459	1412328	11.94%	5.037%
29	6.066	1552	1563	1597	rVB	278996	597062	5.05%	2.129%
30	6.493	1691	1696	1701	rBV5	1046	913	0.01%	0.003%
31	6.548	1711	1713	1721	rVB2	1137	653	0.01%	0.002%
32	6.609	1730	1732	1735	rVB2	705	420	0.00%	0.001%
33	6.773	1781	1783	1787	rVB2	815	446	0.00%	0.002%
34	6.812	1787	1795	1799	rBV6	922	1309	0.01%	0.005%
35	6.841	1802	1804	1805	rBV	666	295	0.00%	0.001%
36	6.879	1814	1816	1818	rBV2	424	187	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027280.D
 Acq On : 11 Aug 2022 12:09
 Operator : SY/MD
 Sample : N4144-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.892	1818	1820	1823	rVB2	570	295	0.00%	0.001%
38	6.924	1828	1830	1832	rBV2	908	433	0.00%	0.002%
39	6.982	1839	1848	1876	rBV	126585	244395	2.07%	0.872%
40	7.313	1940	1951	1973	rBV	412910	747458	6.32%	2.666%
41	7.619	2036	2046	2070	rBV2	93683	177453	1.50%	0.633%
42	7.915	2135	2138	2140	rBV2	434	342	0.00%	0.001%
43	7.950	2144	2149	2151	rBV4	757	731	0.01%	0.003%
44	7.972	2154	2156	2157	rBV	669	302	0.00%	0.001%
45	7.998	2161	2164	2167	rBV3	725	656	0.01%	0.002%
46	8.037	2174	2176	2180	rVB3	1102	515	0.00%	0.002%
47	8.088	2180	2192	2229	rBV	407140	797335	6.74%	2.844%
48	8.718	2384	2388	2389	rBV4	489	368	0.00%	0.001%
49	8.763	2400	2402	2403	rBV2	636	195	0.00%	0.001%
50	8.850	2418	2429	2457	rBV	506287	832009	7.03%	2.967%
51	9.146	2519	2521	2522	rBV	624	281	0.00%	0.001%
52	9.188	2531	2534	2538	rBV5	1038	818	0.01%	0.003%
53	9.210	2539	2541	2544	rBV3	608	396	0.00%	0.001%
54	9.342	2578	2582	2585	rBV3	870	599	0.01%	0.002%
55	9.374	2590	2592	2594	rBV2	344	217	0.00%	0.001%
56	9.561	2649	2650	2654	rVB2	438	307	0.00%	0.001%
57	9.689	2684	2690	2692	rBV2	910	790	0.01%	0.003%
58	9.831	2731	2734	2736	rBV2	499	338	0.00%	0.001%
59	9.882	2747	2750	2753	rBV2	637	404	0.00%	0.001%
60	9.905	2753	2757	2759	rBV4	545	315	0.00%	0.001%
61	10.033	2793	2797	2803	rBV6	1091	1035	0.01%	0.004%
62	10.059	2803	2805	2807	rVB	553	241	0.00%	0.001%
63	10.213	2839	2853	2877	rBV	486556	765451	6.47%	2.730%
64	10.371	2900	2902	2903	rBV	685	202	0.00%	0.001%
65	10.435	2920	2922	2925	rVB2	465	199	0.00%	0.001%
66	10.455	2925	2928	2930	rBV	426	263	0.00%	0.001%
67	10.468	2930	2932	2935	rVB2	518	292	0.00%	0.001%
68	10.586	2966	2969	2972	rVB3	679	432	0.00%	0.002%
69	10.609	2972	2976	2977	rBV3	372	262	0.00%	0.001%
70	10.635	2981	2984	2985	rBV	551	274	0.00%	0.001%
71	10.680	2995	2998	3000	rBV	495	305	0.00%	0.001%
72	10.693	3000	3002	3004	rVV2	399	227	0.00%	0.001%
73	10.705	3004	3006	3009	rVB2	687	304	0.00%	0.001%
74	10.722	3009	3011	3014	rBV3	406	250	0.00%	0.001%
75	10.783	3024	3030	3034	rBV3	748	784	0.01%	0.003%
76	10.821	3039	3042	3044	rBV2	279	208	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
 Data File : VV027280.D
 Acq On : 11 Aug 2022 12:09
 Operator : SY/MD
 Sample : N4144-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.895	3061	3065	3066	rBV3	579	346	0.00%	0.001%
78	11.001	3096	3098	3103	rVB4	728	449	0.00%	0.002%
79	11.043	3106	3111	3112	rBV2	375	261	0.00%	0.001%
80	11.053	3112	3114	3118	rVB2	512	276	0.00%	0.001%
81	11.075	3118	3121	3122	rBV	387	207	0.00%	0.001%
82	11.175	3149	3152	3154	rBV2	511	338	0.00%	0.001%
83	11.246	3163	3174	3186	rBV	442332	689778	5.83%	2.460%
84	11.439	3232	3234	3235	rBV	521	194	0.00%	0.001%
85	11.541	3258	3266	3275	rBV8	3006	6091	0.05%	0.022%
86	11.622	3280	3291	3310	rVV	511125	811271	6.86%	2.893%
87	11.985	3400	3404	3406	rBV3	579	473	0.00%	0.002%
88	11.995	3406	3407	3410	rVB2	746	300	0.00%	0.001%
89	12.069	3429	3430	3433	rVB2	785	206	0.00%	0.001%
90	12.207	3472	3473	3477	rBV4	608	354	0.00%	0.001%
91	12.345	3512	3516	3518	rBV4	753	693	0.01%	0.002%
92	12.635	3604	3606	3608	rBV2	532	258	0.00%	0.001%
93	12.937	3697	3700	3703	rBV4	489	382	0.00%	0.001%
94	13.336	3822	3824	3828	rVB4	828	496	0.00%	0.002%
95	13.506	3875	3877	3879	rBV	627	386	0.00%	0.001%
96	13.744	3946	3951	3956	rBV4	658	872	0.01%	0.003%
97	13.818	3972	3974	3977	rVB2	589	232	0.00%	0.001%
98	14.104	4060	4063	4064	rBV3	631	406	0.00%	0.001%
99	14.384	4148	4150	4152	rBV2	736	373	0.00%	0.001%
100	14.545	4197	4200	4202	rBV2	975	588	0.00%	0.002%




Sum of corrected areas: 28039191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027280.D
Acq On : 11 Aug 2022 12:09
Operator : SY/MD
Sample : N4144-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

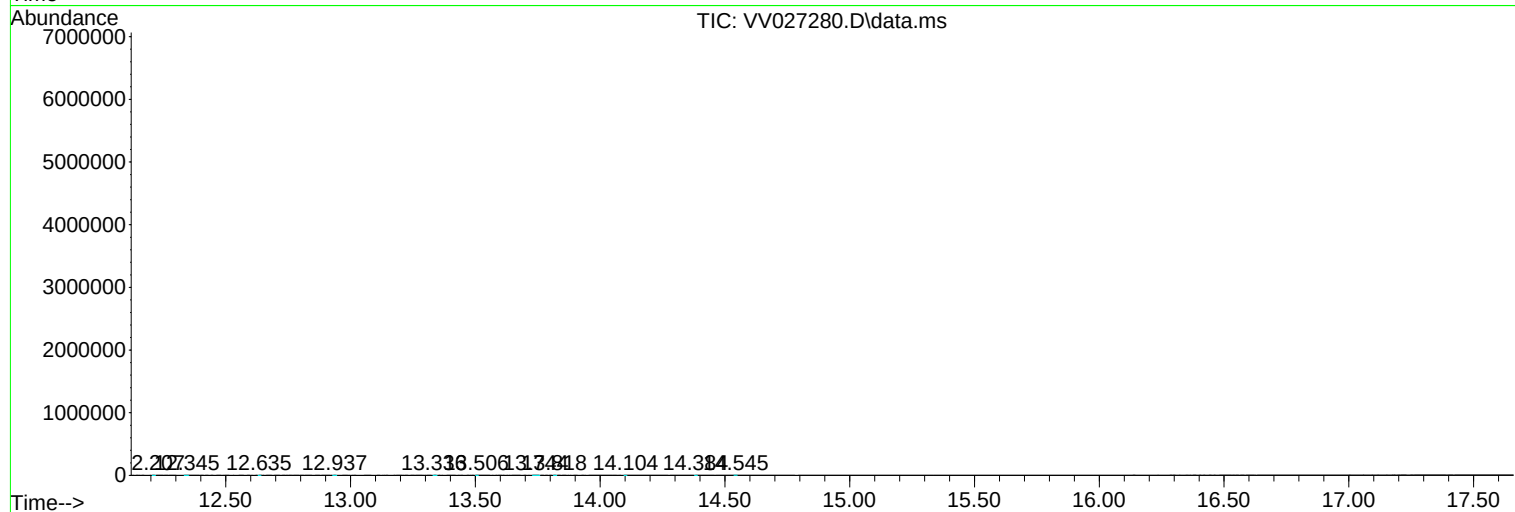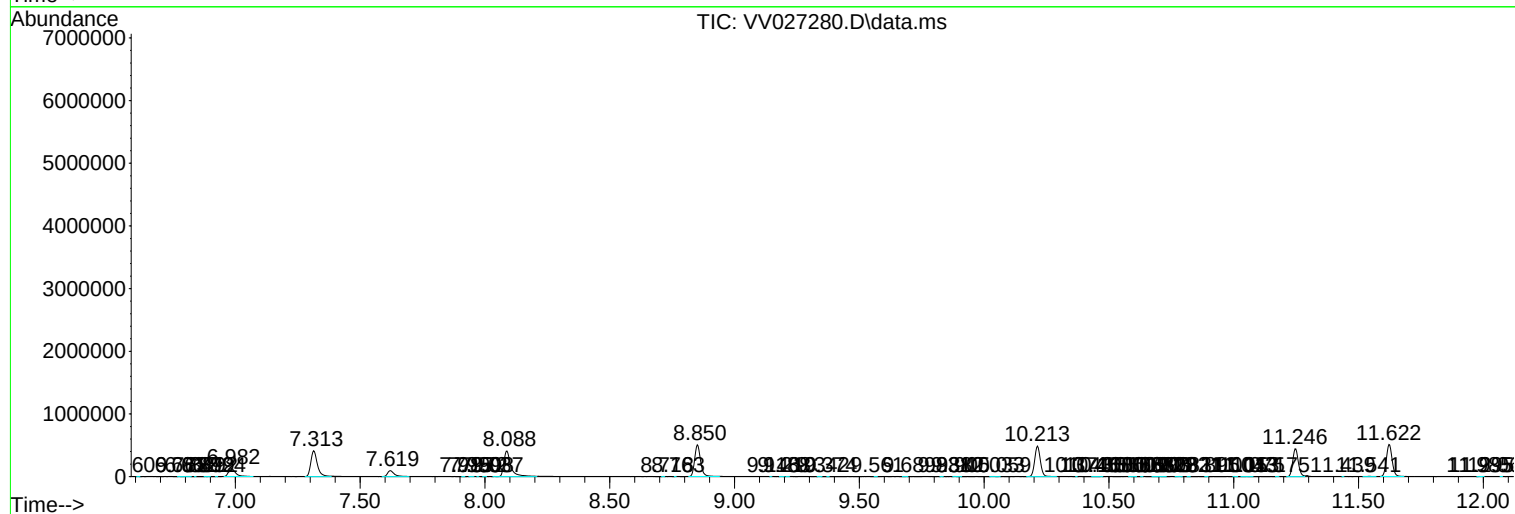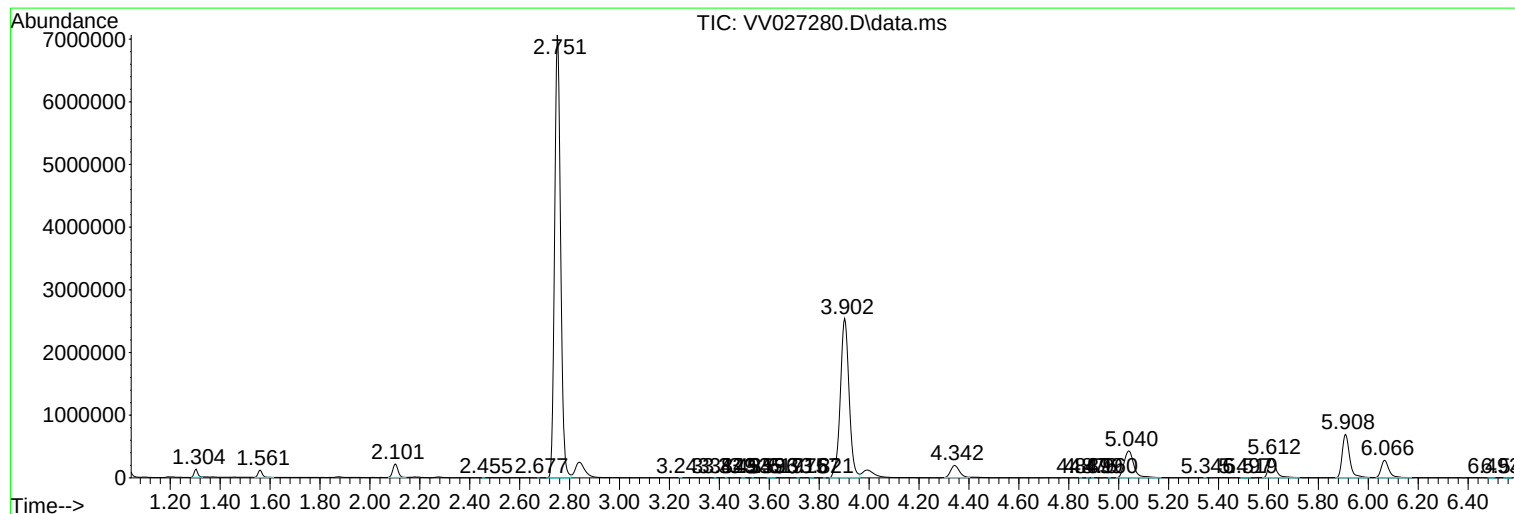

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027280.D
Acq On : 11 Aug 2022 12:09
Operator : SY/MD
Sample : N4144-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027280.D
Acq On : 11 Aug 2022 12:09
Operator : SY/MD
Sample : N4144-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc