
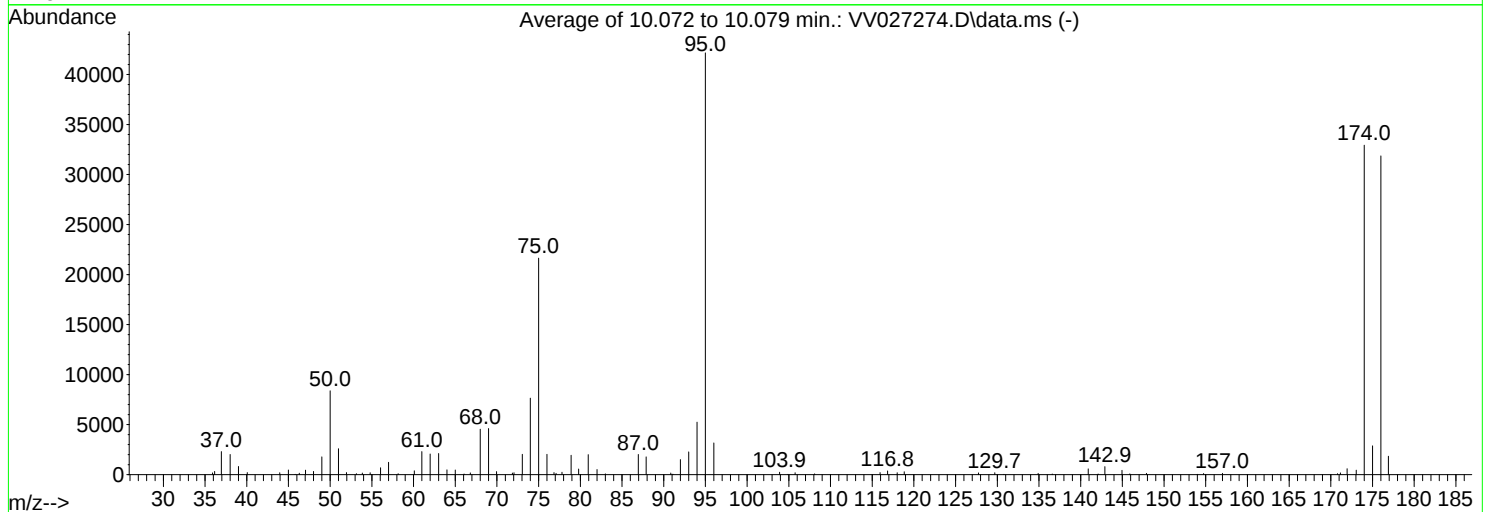


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081122\
Data File : VV027274.D
Acq On : 11 Aug 2022 09:17
Operator : SY/MD
Sample : BFB309
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB309

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Title : VOC Analysis
Last Update : Fri Aug 12 03:40:21 2022

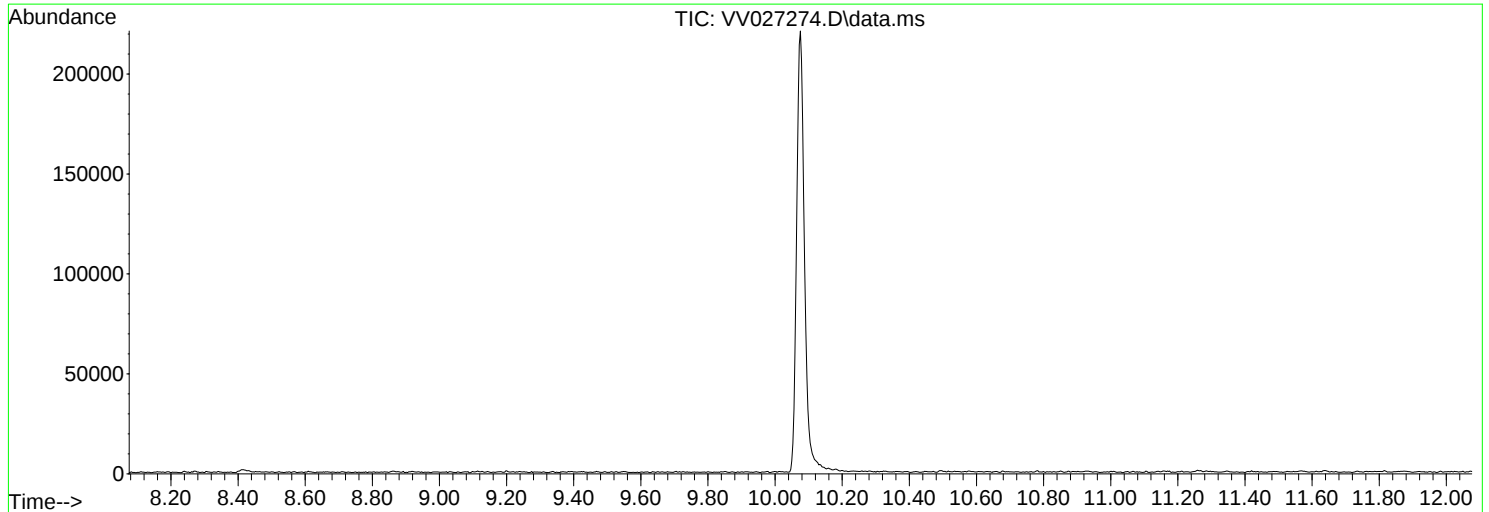

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	8376	PASS
75	95	30	80	51.3	21643	PASS
95	95	100	100	100.0	42165	PASS
96	95	5	9	7.5	3169	PASS
173	174	0.00	2	1.4	456	PASS
174	95	50	120	78.1	32931	PASS
175	174	5	9	8.7	2874	PASS
176	174	95	105	96.8	31861	PASS
177	176	5	10	5.8	1844	PASS

m/z	Abundance
35.20	144.0
39.90	257.0
44.00	500.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.20	439.0
36.90	2377.0
38.00	2066.0
39.10	839.0
39.80	247.0
40.10	271.0
43.90	635.0
45.00	509.0
45.80	108.0
46.30	186.0
47.10	522.0
48.00	349.0
49.00	1885.0
50.00	8188.0
51.00	2624.0
52.00	162.0
53.20	110.0
53.80	185.0
54.80	152.0
56.00	704.0
57.00	1229.0
58.20	109.0
60.10	414.0
61.00	2217.0
62.00	2078.0
63.00	1995.0
64.00	458.0
65.00	524.0
66.10	112.0
66.80	153.0
68.00	4704.0
69.00	4692.0
70.00	335.0
71.80	233.0
73.10	2065.0
74.00	7800.0
75.00	22288.0
76.00	2055.0
76.80	310.0
77.80	245.0
78.90	1958.0
79.80	576.0
81.00	2095.0
82.00	495.0
83.00	121.0
86.90	2013.0
87.90	1980.0
90.90	187.0
92.00	1503.0
93.00	2349.0
94.00	5616.0
95.00	42512.0
96.00	3127.0
103.90	245.0
104.90	103.0
105.70	173.0
115.90	202.0
116.90	311.0
118.00	197.0
118.80	302.0
127.70	214.0
129.70	223.0
134.90	136.0
140.90	564.0
142.90	753.0
144.90	458.0
147.90	136.0
154.70	118.0
156.90	153.0
170.80	138.0
171.20	150.0
171.90	552.0
174.00	32608.0
175.00	2854.0
176.00	31120.0
176.90	1820.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.10	518.0
36.90	2441.0
38.00	2092.0
39.00	837.0
39.90	301.0
43.90	717.0
45.00	455.0
46.30	150.0
47.00	479.0
48.00	322.0
49.00	1743.0
50.00	8755.0
51.00	2660.0
52.00	209.0
53.20	103.0
53.90	157.0
54.80	174.0
56.10	709.0
57.00	1298.0
58.10	103.0
60.10	375.0
61.00	2351.0
62.00	2123.0
63.00	2198.0
64.00	500.0
65.00	500.0
66.00	104.0
66.80	180.0
68.00	4691.0
69.00	4783.0
69.90	314.0
71.90	270.0
72.10	266.0
73.00	2080.0
74.00	7894.0
75.00	22296.0
76.00	2117.0
76.90	334.0
77.80	235.0
78.90	1977.0
79.80	565.0
81.00	2039.0
82.00	500.0
83.00	112.0
86.90	2060.0
87.90	1786.0
90.90	178.0
92.00	1561.0
93.00	2400.0
94.00	5398.0
95.00	43536.0
96.00	3309.0
103.90	255.0
105.80	190.0
108.10	124.0
116.00	218.0
116.80	373.0
118.00	202.0
118.90	280.0
127.70	178.0
129.70	202.0
134.90	133.0
136.60	109.0
140.90	592.0
142.10	102.0
142.90	840.0
144.90	460.0
145.90	118.0
147.90	149.0
154.70	129.0
157.00	138.0
170.80	153.0
171.20	180.0
172.00	572.0
173.10	673.0
174.00	33936.0
175.00	2991.0
176.00	33056.0
176.90	1888.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
35.90	524.0
37.00	2114.0
38.00	1903.0
38.90	791.0
40.00	370.0
44.00	718.0
45.00	415.0
46.20	105.0
47.00	345.0
48.00	285.0
49.00	1695.0
50.00	8186.0
51.00	2476.0
51.90	247.0
53.10	103.0
53.90	121.0
54.80	234.0
56.10	647.0
57.00	1192.0
58.10	104.0
60.10	350.0
61.00	2339.0
62.00	1991.0
63.00	2146.0
64.00	488.0
65.00	391.0
66.80	178.0
68.00	4251.0
69.00	4350.0
70.00	287.0
72.00	294.0
73.00	1964.0
74.00	7248.0
75.00	20344.0
76.00	1903.0
77.10	398.0
77.80	228.0
78.90	1888.0
79.80	523.0
80.90	1884.0
82.00	536.0
87.00	1995.0
87.90	1551.0
90.80	141.0
91.10	142.0
92.00	1466.0
93.00	2058.0
94.00	4709.0
95.00	40448.0
96.00	3071.0
103.90	244.0
105.80	197.0
108.10	113.0
115.90	203.0
116.80	424.0
118.00	174.0
118.90	271.0
127.80	147.0
129.70	166.0
130.80	123.0
134.90	119.0
136.60	102.0
140.90	569.0
142.10	101.0
142.90	813.0
145.00	405.0
145.90	132.0
147.90	103.0
154.00	106.0
154.80	112.0
157.10	105.0
171.10	202.0
172.00	635.0
173.00	695.0
174.00	32248.0
175.00	2778.0
176.00	31408.0
176.90	1824.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309