


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081123\
Data File : VV031790.D
Acq On : 11 Aug 2023 08:27
Operator : SY/MD
Sample : BFB285
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB285

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Aug 12 05:18:45 2023

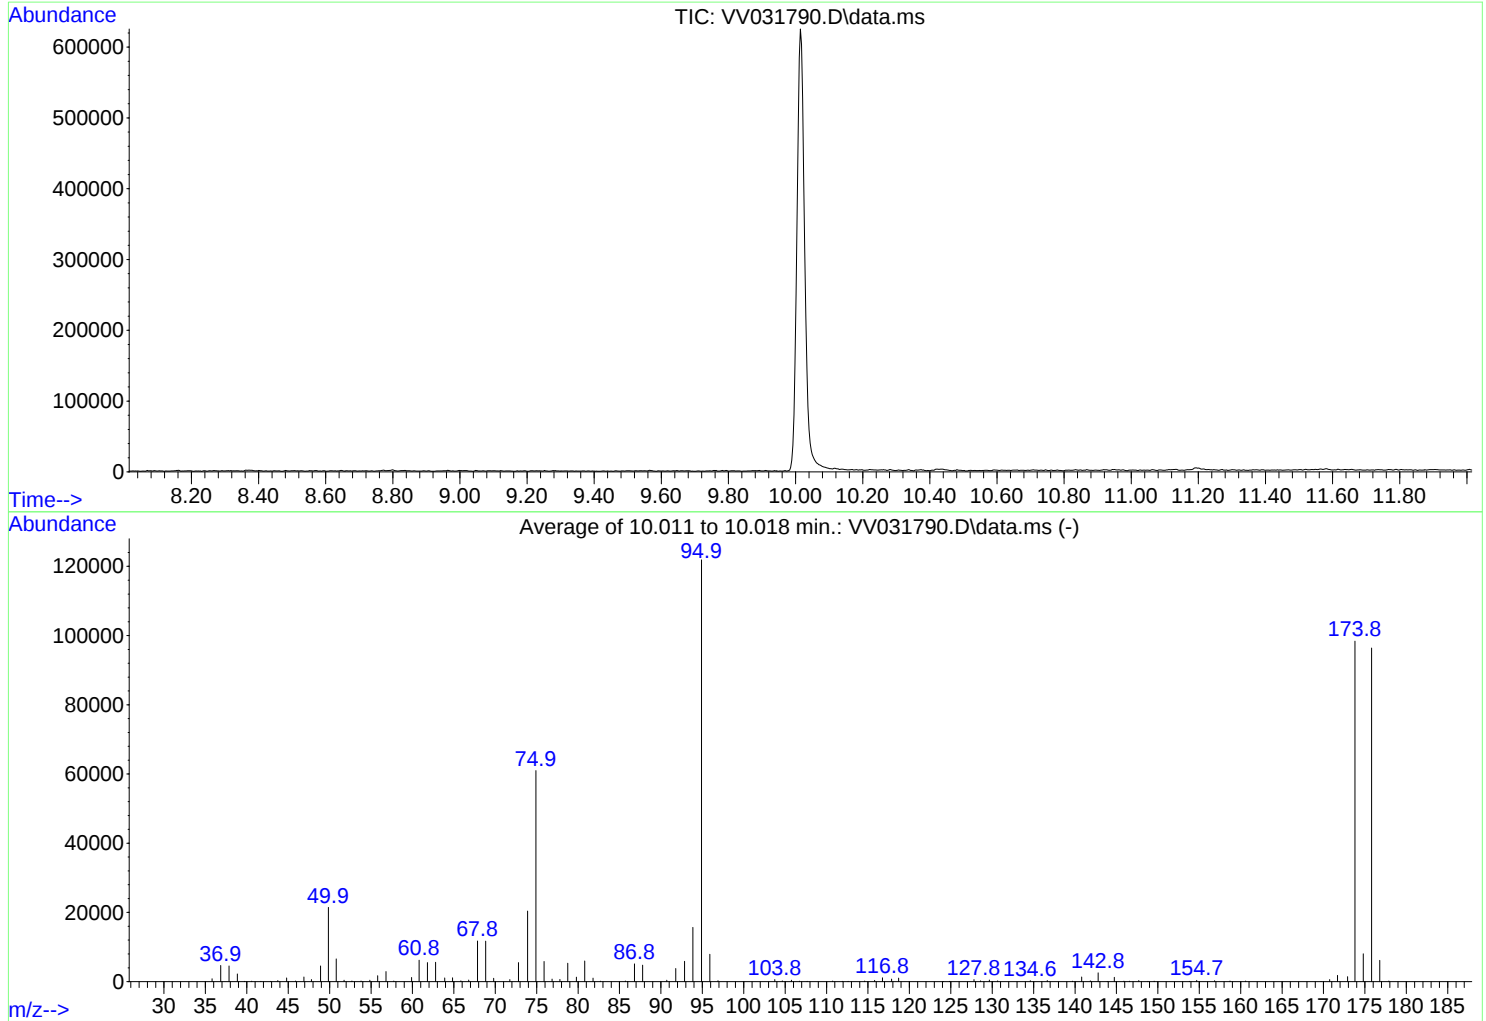

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	21440	PASS
75	95	30	80	50.0	60971	PASS
95	95	100	100	100.0	121880	PASS
96	95	5	9	6.5	7931	PASS
173	174	0.00	2	1.5	1448	PASS
174	95	50	120	80.7	98395	PASS
175	174	5	9	8.2	8025	PASS
176	174	95	105	98.0	96392	PASS
177	176	5	10	6.4	6160	PASS

m/z	Abundance
35.80	109.0
38.00	101.0
39.80	403.0
41.00	178.0
43.80	748.0
47.80	105.0
72.70	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
35.80	920.0
36.80	4586.0
37.80	4938.0
38.80	2054.0
39.80	431.0
40.60	226.0
41.70	113.0
42.80	115.0
43.70	1066.0
44.80	1131.0
45.90	249.0
46.90	1442.0
47.80	700.0
48.90	4704.0
49.90	21280.0
50.80	6779.0
51.80	375.0
52.70	147.0
53.80	238.0
54.90	413.0
55.80	1494.0
56.80	2792.0
57.70	172.0
59.90	1087.0
60.80	6108.0
61.80	5466.0
62.80	5301.0
63.90	997.0
64.90	1065.0
65.90	233.0
66.80	566.0
67.90	11628.0
68.80	11322.0
69.80	898.0
71.80	587.0
72.90	5395.0
73.90	20504.0
74.90	60216.0
75.90	6025.0
76.90	715.0
77.70	586.0
78.80	5127.0
79.80	1328.0
80.80	5580.0
81.80	1016.0
82.70	116.0
85.70	295.0
86.80	5123.0
87.80	4650.0
90.80	493.0
91.80	3985.0
92.90	5345.0
93.90	15301.0
94.90	117520.0
95.90	7854.0
96.80	246.0
103.70	586.0
104.70	227.0
105.70	478.0
106.70	123.0
110.70	206.0
112.50	131.0
114.70	195.0
115.80	314.0
116.70	1146.0
117.80	677.0
118.70	1002.0
124.80	136.0
127.80	553.0
128.60	234.0
129.60	417.0
130.60	229.0
134.60	280.0
136.70	268.0
139.70	198.0
140.80	1176.0
142.00	183.0
142.80	2409.0
143.90	107.0
144.80	1217.0
145.90	104.0
146.60	144.0
147.70	296.0
149.60	109.0
153.80	181.0
154.70	300.0
156.80	207.0
158.70	119.0
160.50	129.0
170.70	614.0
171.70	1516.0
172.90	1310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

173.80	94208.0
174.80	7683.0
175.80	90456.0
176.80	5988.0
177.90	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
35.80	947.0
36.90	4647.0
37.90	4358.0
38.90	2310.0
39.70	520.0
41.70	104.0
43.80	1135.0
44.80	1014.0
46.90	1248.0
47.90	670.0
48.90	4226.0
49.80	21008.0
50.80	6228.0
51.70	505.0
52.70	220.0
53.90	123.0
54.80	400.0
55.80	1818.0
56.80	2932.0
57.80	160.0
59.90	1264.0
60.80	6069.0
61.80	5383.0
62.80	5674.0
63.90	1127.0
64.80	1145.0
65.80	188.0
66.90	314.0
67.80	11585.0
68.90	11802.0
69.80	1008.0
71.70	613.0
72.80	5606.0
73.90	19664.0
74.90	59664.0
75.90	5359.0
76.80	779.0
77.90	694.0
78.70	5353.0
79.80	1184.0
80.80	6085.0
81.80	1007.0
82.70	177.0
86.00	204.0
86.80	4929.0
87.80	4795.0
90.60	397.0
91.80	3564.0
92.80	6168.0
93.80	15459.0
94.90	121920.0
95.90	7711.0
97.00	293.0
103.80	568.0
104.70	220.0
105.80	404.0
106.80	167.0
107.70	228.0
110.70	146.0
111.90	182.0
112.70	112.0
114.50	167.0
115.80	450.0
116.80	1124.0
117.90	696.0
118.70	981.0
124.10	102.0
127.80	590.0
128.60	246.0
129.70	499.0
130.70	277.0
134.60	268.0
136.60	351.0
140.80	1503.0
141.70	248.0
142.80	2541.0
143.90	100.0
144.70	1250.0
145.90	164.0
146.60	106.0
147.70	338.0
148.80	222.0
149.50	156.0
154.70	441.0
156.90	309.0
158.70	282.0
160.70	216.0
169.70	110.0
170.80	551.0
171.70	2010.0
172.90	1559.0
173.80	99248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

174.80	8046.0
175.80	98824.0
176.80	6019.0
177.90	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
35.80	982.0
36.90	4796.0
37.90	4627.0
38.90	2250.0
39.80	524.0
40.60	169.0
41.70	138.0
42.90	120.0
43.80	1075.0
44.80	1089.0
45.90	285.0
46.90	1374.0
47.80	726.0
48.90	4617.0
49.80	22032.0
50.80	6713.0
51.80	440.0
52.70	184.0
53.80	187.0
54.90	405.0
55.80	1826.0
56.80	3040.0
57.70	198.0
59.90	1244.0
60.80	6367.0
61.80	5652.0
62.80	5864.0
63.90	1082.0
64.90	1177.0
65.80	226.0
66.80	502.0
67.80	12049.0
68.90	12031.0
69.80	1026.0
71.70	647.0
72.80	5819.0
73.90	20984.0
74.90	63032.0
75.90	6080.0
76.80	731.0
77.80	612.0
78.80	5516.0
79.80	1336.0
80.80	6204.0
81.80	1042.0
82.70	177.0
85.70	237.0
86.80	5345.0
87.80	4871.0
90.70	427.0
91.80	3888.0
92.80	6174.0
93.80	16327.0
94.90	126200.0
95.90	8229.0
96.90	284.0
103.70	651.0
104.60	228.0
105.80	448.0
106.80	132.0
107.60	122.0
110.80	171.0
111.90	103.0
112.60	111.0
114.60	200.0
115.80	310.0
116.80	1135.0
117.80	794.0
118.70	1047.0
124.90	142.0
127.80	658.0
128.60	266.0
129.70	481.0
130.70	255.0
134.60	290.0
136.60	364.0
139.70	162.0
140.80	1420.0
141.80	240.0
142.80	2637.0
144.70	1306.0
145.90	136.0
146.60	116.0
147.70	321.0
148.80	121.0
149.50	166.0
153.80	144.0
154.70	420.0
156.90	279.0
158.70	213.0
160.60	156.0
170.70	657.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

171.70	1839.0
172.90	1474.0
173.80	101728.0
174.80	8346.0
175.80	99896.0
176.80	6473.0
177.90	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285