


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV081125\
Data File : VV038935.D
Acq On : 11 Aug 2025 08:29
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V080825W.M
Title : SW846 8260
Last Update : Mon Aug 11 05:27:06 2025

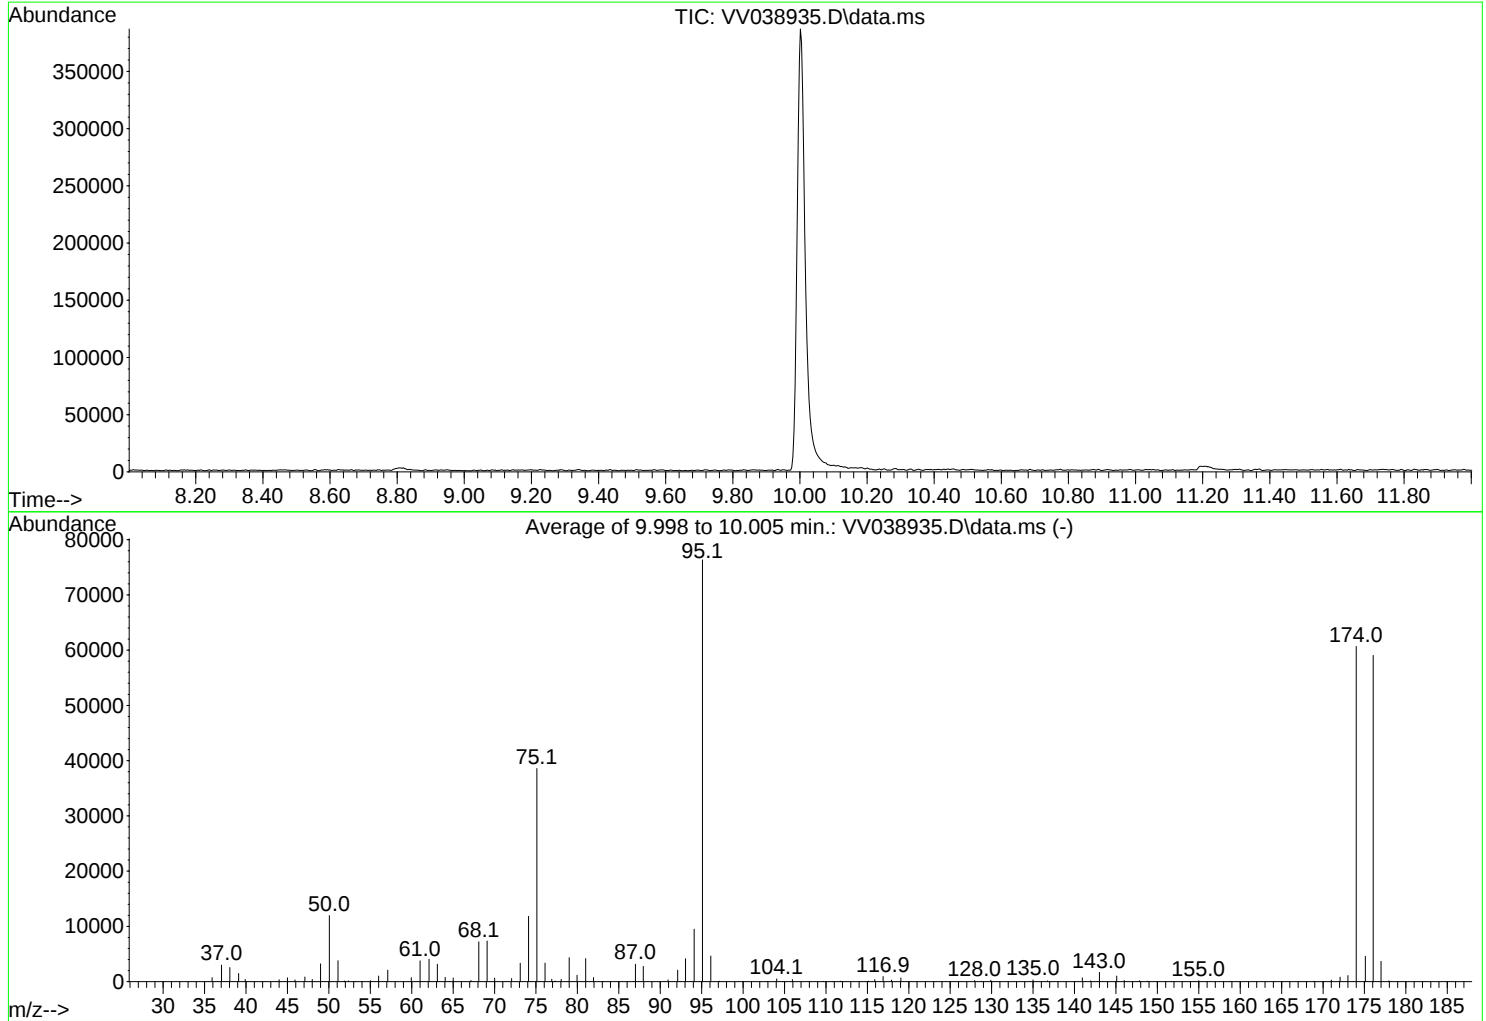

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	11954	PASS
75	95	30	60	50.5	38565	PASS
95	95	100	100	100.0	76349	PASS
96	95	5	9	6.1	4635	PASS
173	174	0.00	2	1.8	1089	PASS
174	95	50	100	79.5	60667	PASS
175	174	5	9	7.6	4590	PASS
176	174	95	101	97.3	59045	PASS
177	176	5	9	6.3	3691	PASS