

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081219\
 Data File : VV012210.D
 Acq On : 12 Aug 2019 17:18
 Operator : SY/MD
 Sample : K4248-20
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2B63

Quant Time: Aug 13 07:01:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 13 06:45:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	392650	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	377027	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	169053	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	139337	53.93	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	107.86%
7) Chloroethane-d5	1.58	69	131433	58.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	116.28%
11) 1,1-Dichloroethene-d2	2.13	63	197340	40.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.56%
21) 2-Butanone-d5	3.92	46	301260	131.89	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	131.89%#
24) Chloroform-d	4.40	84	336317	57.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	114.70%
26) 1,2-Dichloroethane-d4	5.08	65	225288	60.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	120.78%
32) Benzene-d6	5.10	84	689185	57.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.94%
36) 1,2-Dichloropropane-d6	6.12	67	221914	60.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	120.36%#
41) Toluene-d8	7.36	98	609328	56.58	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.16%
43) trans-1,3-Dichloropropene-	7.66	79	103472	55.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	111.16%
47) 2-Hexanone-d5	8.13	63	200189	124.24	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	124.24%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	315416	58.84	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	117.68%
64) 1,2-Dichlorobenzene-d4	11.67	152	248047	61.47	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	122.94%#


Target Compounds					Ovalue
13) Acetone	2.19	43	25123	13.905 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081219\
Data File : VV012210.D
Acq On : 12 Aug 2019 17:18
Operator : SY/MD
Sample : K4248-20
Misc : 5mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2B63

Quant Time: Aug 13 07:01:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081219WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 13 06:45:02 2019
Response via : Initial Calibration

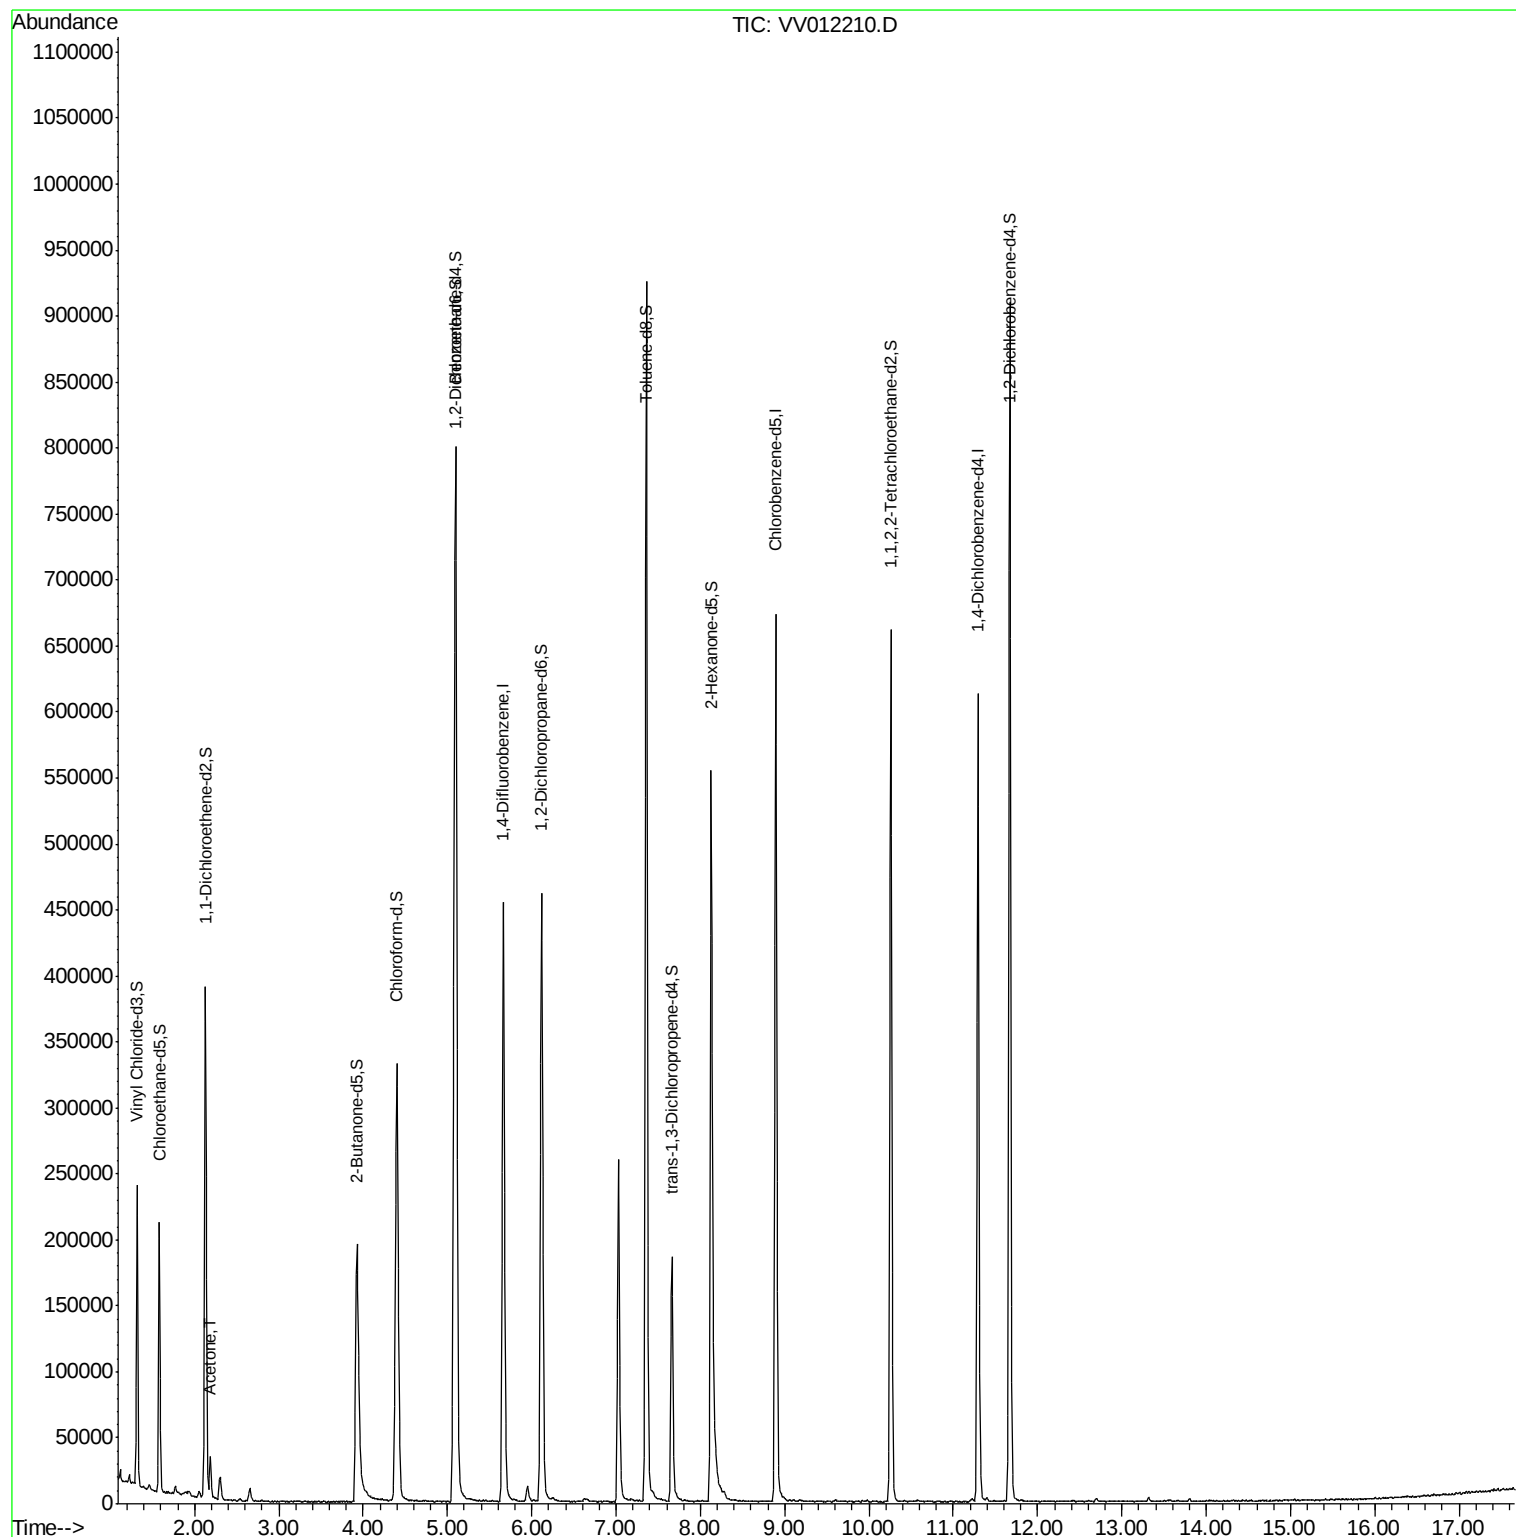

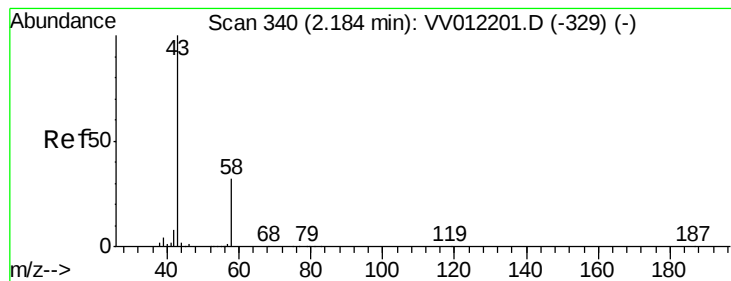

#13

Acetone

Concen: 13.905 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.00 min

Lab File: VV012210.D

Acq: 12 Aug 2019 17:18

Instrument :
MSVOA_V
ClientSampleId :
F2B63

Tot Ion: 43 Resp: 25123

Ion Ratio Lower Upper

43 100

58 30.6 0.0 63.2

