


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081219\
Data File : VV012197.D
Acq On : 12 Aug 2019 08:37
Operator : SY/MD
Sample : BFB65
Misc : 5mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081219WMA.M
Title : VOC Analysis
Last Update : Tue Aug 13 10:20:00 2019

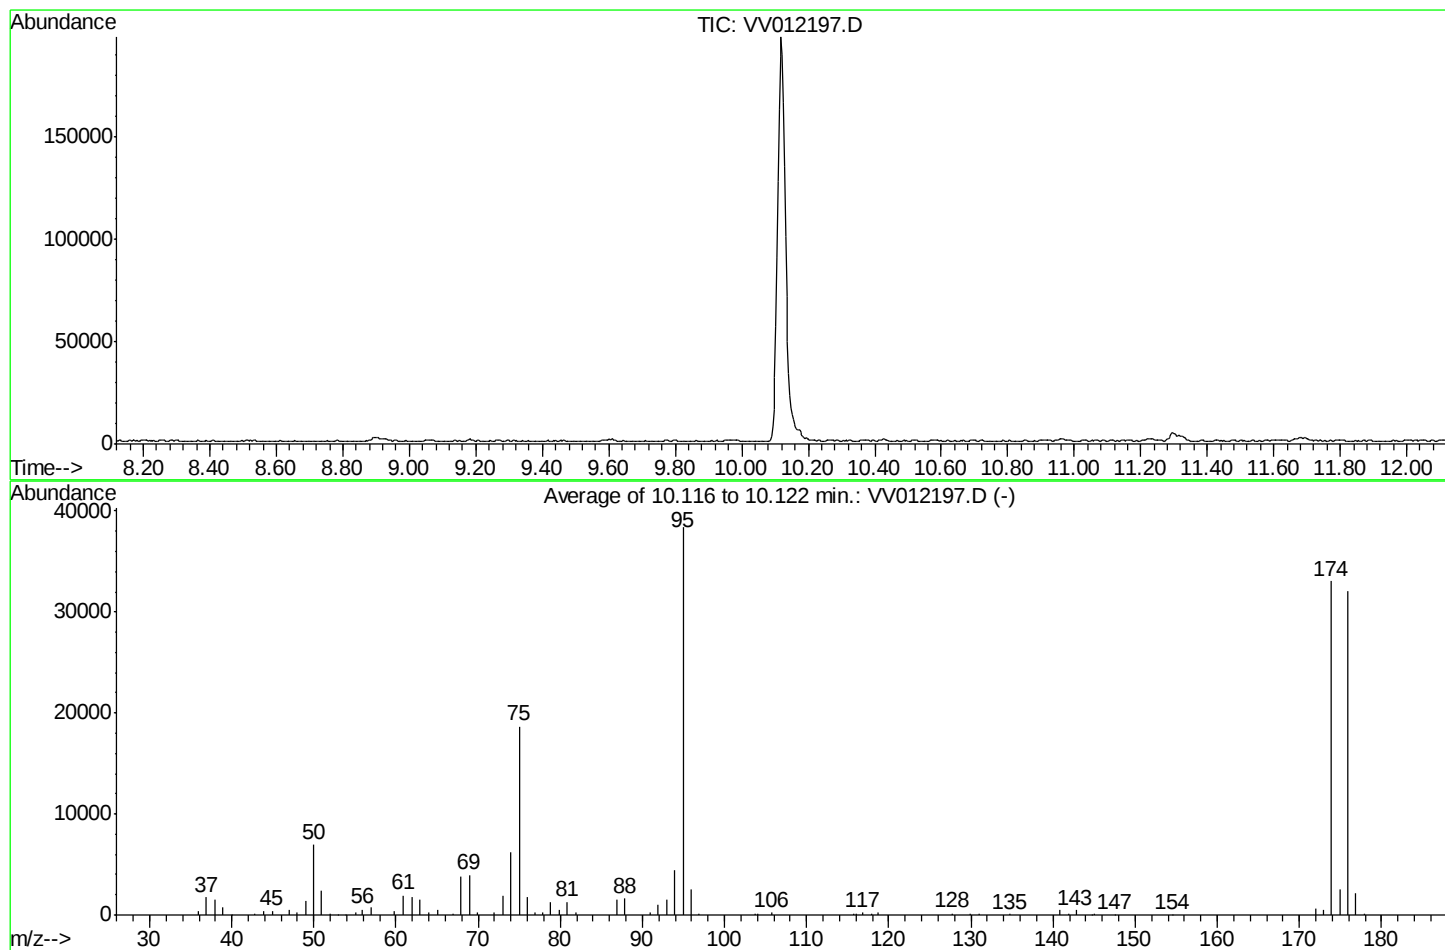

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	6932	PASS
75	95	30	80	48.5	18632	PASS
95	95	100	100	100.0	38386	PASS
96	95	5	9	6.7	2586	PASS
173	174	0.00	2	1.5	482	PASS
174	95	50	120	86.1	33058	PASS
175	174	5	9	7.8	2564	PASS
176	174	95	101	96.9	32037	PASS
177	176	5	9	6.6	2102	PASS

m/z	Abundance
35.90	380.0
36.90	1769.0
37.90	1602.0
39.00	766.0
39.90	777.0
43.90	927.0
44.90	395.0
47.00	410.0
48.00	228.0
49.00	1419.0
50.00	6819.0
50.90	2449.0
51.90	150.0
52.90	124.0
55.10	155.0
55.90	574.0
56.90	869.0
59.80	372.0
60.90	2030.0
62.00	1710.0
63.00	1548.0
63.90	239.0
65.00	509.0
67.00	155.0
67.90	3864.0
69.00	4129.0
70.00	303.0
72.00	242.0
73.00	1791.0
74.00	6303.0
75.00	18752.0
76.00	1803.0
77.00	298.0
77.80	225.0
78.80	1301.0
79.80	441.0
80.80	1302.0
81.90	342.0
86.90	1525.0
87.80	1533.0
90.80	207.0
91.90	1008.0
92.90	1622.0
93.90	4390.0
95.00	37568.0
96.00	2547.0
96.90	117.0
103.80	229.0
105.80	189.0
116.90	249.0
117.90	151.0
118.80	259.0
127.80	180.0
129.90	138.0
131.00	119.0
140.90	477.0
141.90	100.0
142.80	483.0
145.00	178.0
171.90	600.0
173.00	457.0
173.90	32072.0
174.90	2553.0
175.90	30312.0
176.90	2141.0
177.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	438.0
36.90	1763.0
37.90	1509.0
38.90	771.0
39.90	750.0
42.80	118.0
43.90	917.0
44.90	396.0
47.00	522.0
47.90	278.0
49.00	1517.0
50.00	7142.0
50.90	2547.0
51.90	154.0
55.10	214.0
55.90	558.0
56.90	822.0
59.80	364.0
60.90	2021.0
61.90	1820.0
63.00	1609.0
63.90	278.0
65.00	551.0
67.00	115.0
67.90	3925.0
68.90	4132.0
69.90	311.0
72.00	225.0
72.90	1947.0
74.00	6342.0
75.00	19208.0
76.00	1824.0
76.90	312.0
77.80	247.0
78.80	1368.0
79.80	466.0
80.80	1317.0
81.80	302.0
86.90	1635.0
87.90	1621.0
90.90	206.0
92.00	1082.0
92.90	1564.0
93.90	4655.0
95.00	39552.0
96.00	2687.0
96.90	120.0
103.80	214.0
105.80	203.0
115.70	108.0
116.00	110.0
116.80	238.0
117.90	146.0
118.70	206.0
127.80	168.0
129.90	140.0
131.00	114.0
134.80	138.0
140.90	474.0
141.90	116.0
142.80	496.0
145.00	170.0
154.60	100.0
171.90	636.0
172.90	491.0
173.90	34104.0
174.90	2655.0
175.90	33072.0
176.90	2174.0
177.90	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	421.0
36.90	1658.0
37.90	1335.0
38.90	682.0
39.90	826.0
42.80	114.0
43.90	840.0
44.90	405.0
46.90	558.0
47.90	271.0
48.90	1443.0
50.00	6837.0
50.90	2309.0
51.90	124.0
53.90	107.0
55.00	221.0
56.00	496.0
57.00	743.0
59.80	314.0
60.90	1762.0
61.90	1850.0
62.90	1535.0
63.90	290.0
65.00	482.0
67.90	3559.0
68.90	3698.0
69.90	286.0
72.00	217.0
72.90	1833.0
74.00	5909.0
75.00	17936.0
76.00	1770.0
77.00	310.0
77.80	256.0
78.80	1202.0
79.80	440.0
80.90	1249.0
81.80	262.0
86.90	1585.0
88.00	1686.0
91.00	196.0
91.90	1030.0
92.90	1460.0
93.90	4341.0
95.00	38040.0
96.00	2525.0
96.90	136.0
104.00	208.0
105.80	220.0
115.70	118.0
116.00	109.0
116.80	231.0
117.90	163.0
118.80	187.0
127.80	136.0
129.80	144.0
134.80	138.0
140.90	435.0
141.80	103.0
142.90	511.0
144.70	155.0
147.60	104.0
172.00	599.0
173.00	499.0
173.90	33000.0
174.90	2486.0
175.90	32728.0
176.90	1992.0
177.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Scan 2796 (10.080 min): VV012197.D
BFB65

m/z	Abundance
39.90	736.0
43.90	509.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65