

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081220\
 Data File : VV017925.D
 Acq On : 12 Aug 2020 14:03
 Operator : SY/MD
 Sample : L3644-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L29

Quant Time: Aug 13 05:04:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 13 04:34:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	260169	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	249965	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	110257	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	93217	46.96	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.92%
7) Chloroethane-d5	1.58	69	78941	48.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.22%
11) 1,1-Dichloroethene-d2	2.12	63	138578	36.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.00%
21) 2-Butanone-d5	3.91	46	127032	97.71	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.71%
24) Chloroform-d	4.38	84	171475	47.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.90%
26) 1,2-Dichloroethane-d4	5.06	65	118192	50.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.72%
32) Benzene-d6	5.07	84	345840	50.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.40%
36) 1,2-Dichloropropane-d6	6.09	67	113144	50.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.48%
41) Toluene-d8	7.34	98	303577	49.00	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.00%
43) trans-1,3-Dichloropropene-	7.64	79	48542	47.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.04%
47) 2-Hexanone-d5	8.11	63	67662	93.62	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.62%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	140317	47.84	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.68%
64) 1,2-Dichlorobenzene-d4	11.65	152	116969	53.90	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.80%


Target Compounds				Ovalue
13) Acetone	2.20	43	1664	1.239 ug/L 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081220\
Data File : VV017925.D
Acq On : 12 Aug 2020 14:03
Operator : SY/MD
Sample : L3644-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L29

Quant Time: Aug 13 05:04:18 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 13 04:34:59 2020
Response via : Initial Calibration

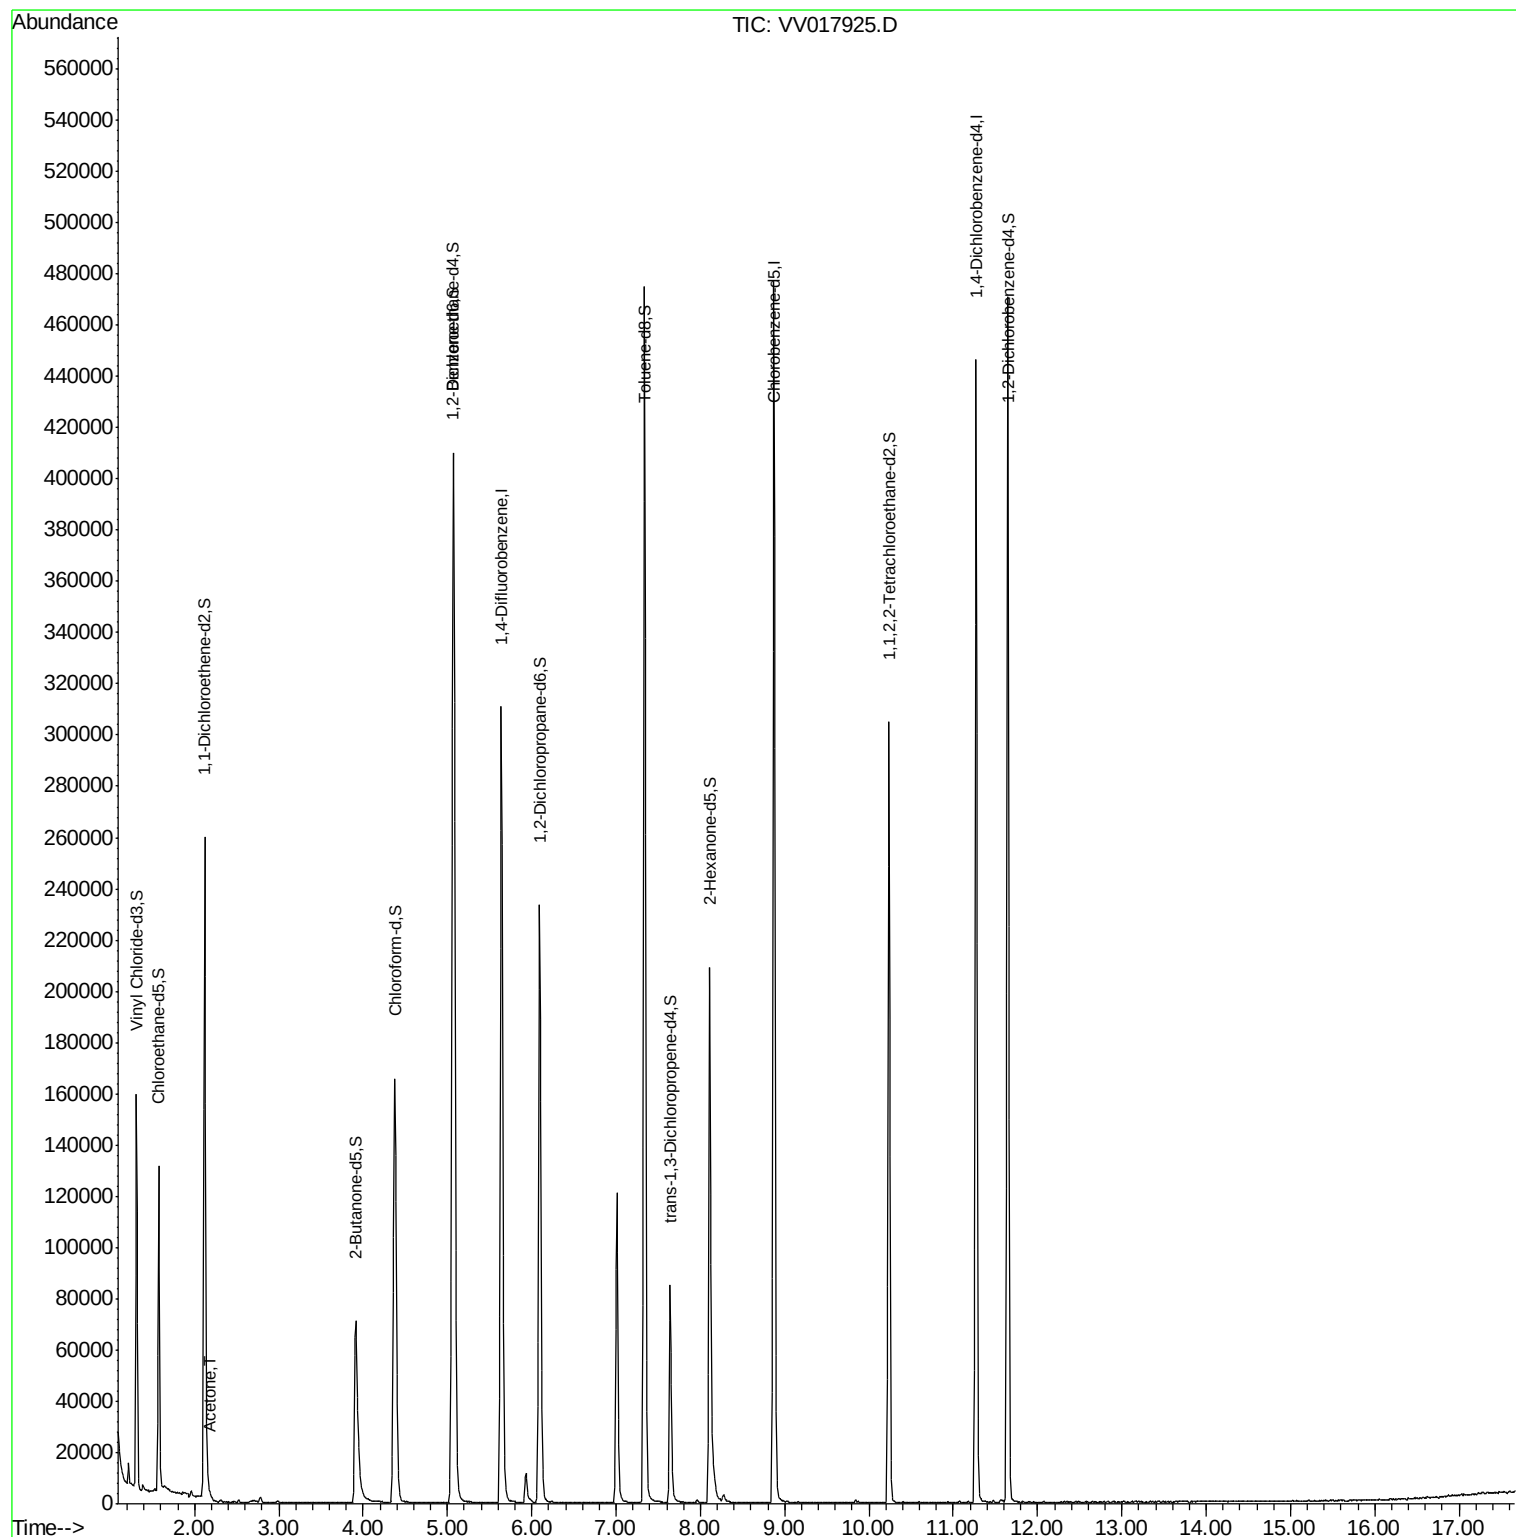

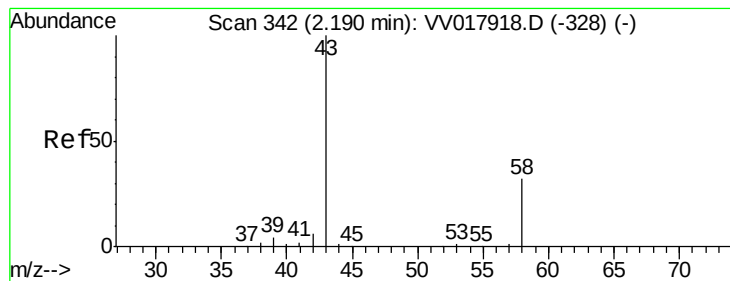

#13

Acetone

Concen: 1.239 ug/L

RT: 2.20 min Scan# 344

Delta R.T. 0.01 min

Lab File: VV017925.D

Acq: 12 Aug 2020 14:03

Instrument :
MSVOA_V
ClientSampleId :
F4L29

Tot Ion: 43 Resp: 1664

Ion Ratio Lower Upper

43 100

58 22.5 0.0 63.6

