

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081220\
 Data File : VV017927.D
 Acq On : 12 Aug 2020 14:50
 Operator : SY/MD
 Sample : L3644-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2L60

Quant Time: Aug 13 05:11:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 13 04:34:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	255032	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	247166	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	109991	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	88606	45.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.08%
7) Chloroethane-d5	1.58	69	75344	47.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.66%
11) 1,1-Dichloroethene-d2	2.12	63	130655	35.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.20%
21) 2-Butanone-d5	3.91	46	129708	101.77	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.77%
24) Chloroform-d	4.38	84	166031	46.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.74%
26) 1,2-Dichloroethane-d4	5.06	65	114823	49.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.82%
32) Benzene-d6	5.07	84	333262	48.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.84%
36) 1,2-Dichloropropane-d6	6.09	67	111010	49.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.70%
41) Toluene-d8	7.34	98	292333	47.72	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.44%
43) trans-1,3-Dichloropropene-	7.64	79	46726	46.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.52%
47) 2-Hexanone-d5	8.11	63	72013	100.77	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.77%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	137222	47.32	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.64%
64) 1,2-Dichlorobenzene-d4	11.65	152	114679	52.98	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.96%

Target Compounds


					Ovalue
5) Vinyl chloride	1.32	62	90212	39.809	ug/L 97
8) Chloroethane	1.60	64	2838	1.962	ug/L 96
17) trans-1,2-Dichloroethene	2.78	96	8624	4.904	ug/L 99
20) cis-1,2-Dichloroethene	3.94	96	751167	388.706	ug/L 99
34) Trichloroethene	5.94	95	1924285	952.003	ug/L 99
46) Tetrachloroethene	8.00	164	898455	606.078	ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081220\
Data File : VV017927.D
Acq On : 12 Aug 2020 14:50
Operator : SY/MD
Sample : L3644-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2L60

Quant Time: Aug 13 05:11:38 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 13 04:34:59 2020
Response via : Initial Calibration

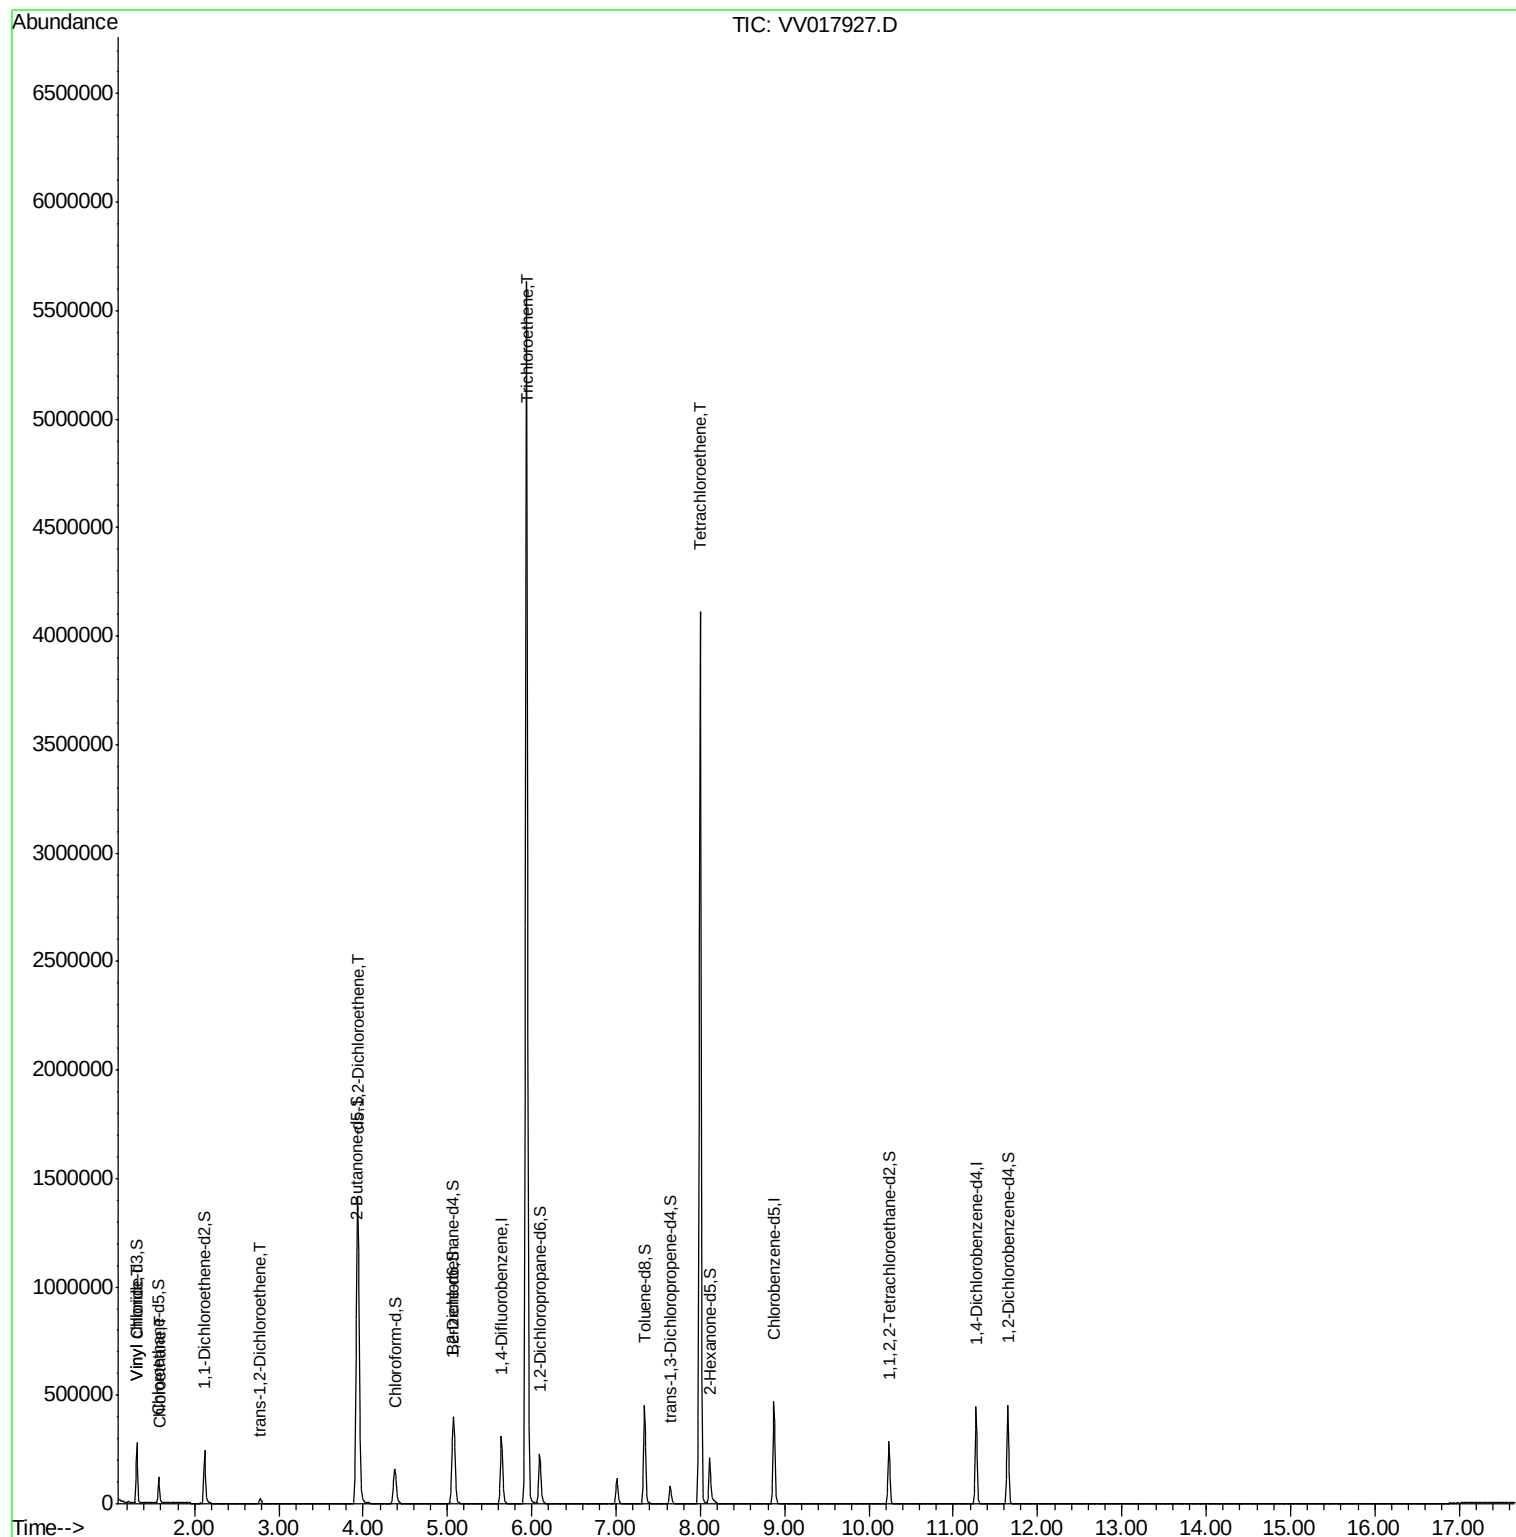

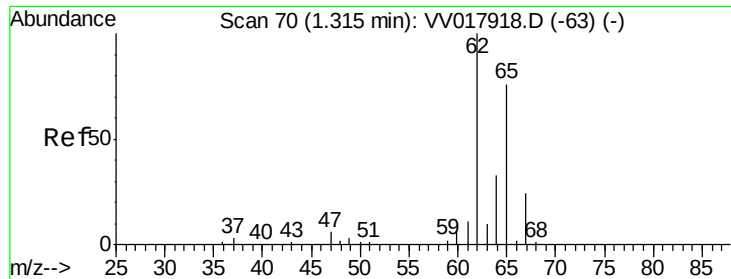

#5

Vinyl chloride

Concen: 39.809 ug/L

RT: 1.32 min Scan# 71

Delta R.T. 0.00 min

Lab File: VV017927.D

Acq: 12 Aug 2020 14:50

Instrument :

MSVOA_V

ClientSampleId :





F2L60

Tot Ion: 62 Resp: 90212

Ion Ratio Lower Upper

62 100

64 33.4 22.4 41.6

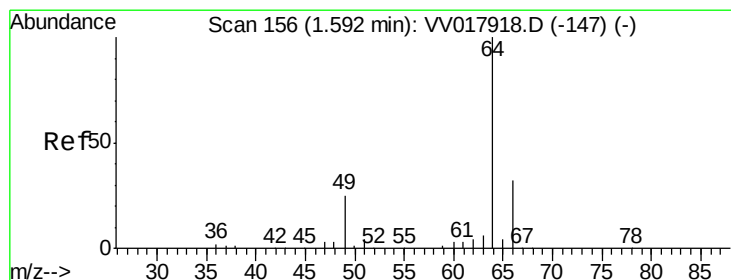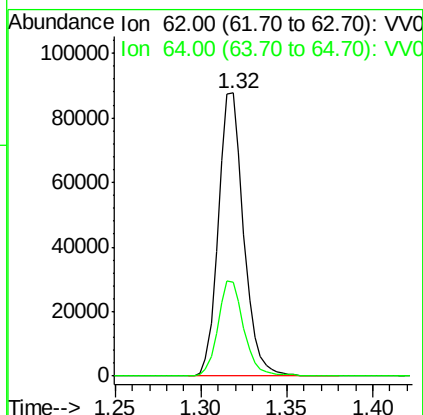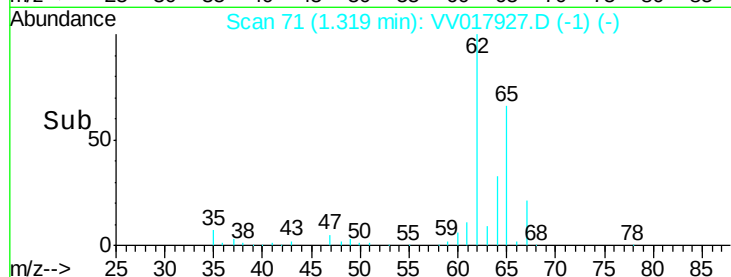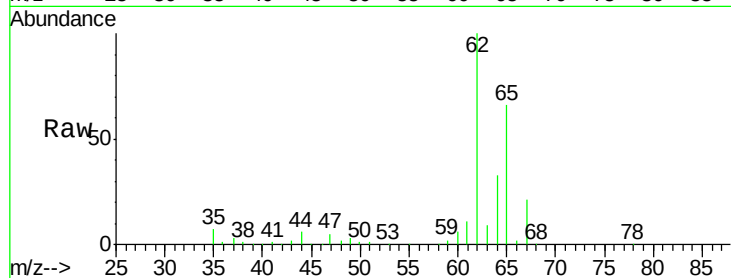

#8

Chloroethane

Concen: 1.962 ug/L

RT: 1.60 min Scan# 157

Delta R.T. 0.00 min

Lab File: VV017927.D




Acq: 12 Aug 2020 14:50


Tgt Ion: 64 Resp: 2838

Ion Ratio Lower Upper

64 100

66 29.4 22.3 41.3

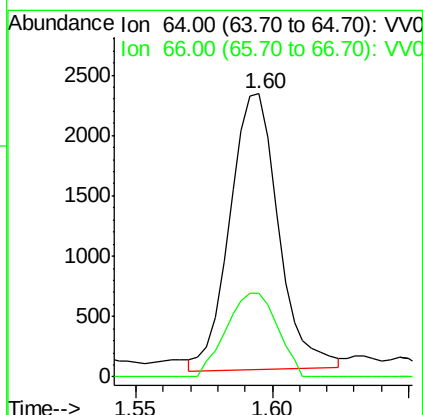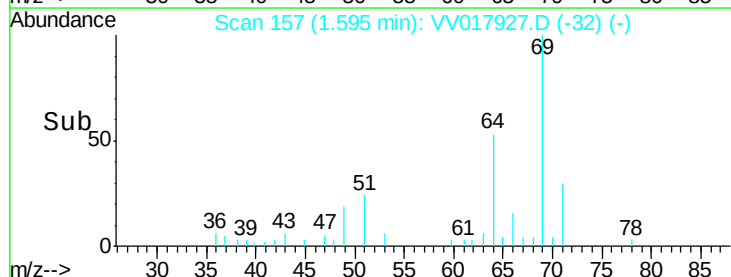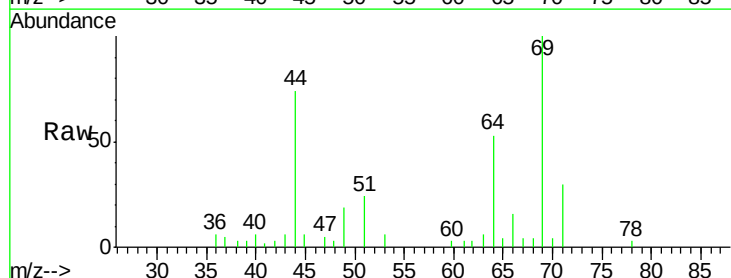

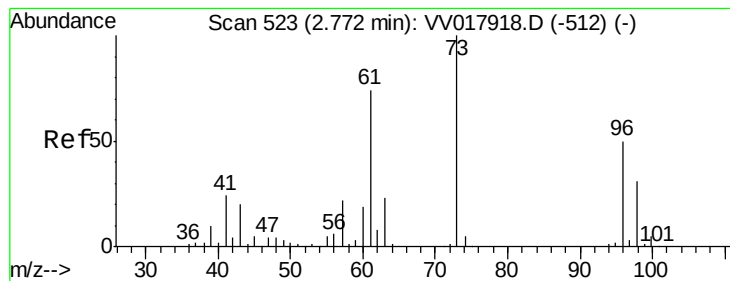

#17

trans-1,2-Dichloroethene

Concen: 4.904 ug/L

RT: 2.78 min Scan# 525

Delta R.T. 0.01 min

Lab File: VV017927.D

Acq: 12 Aug 2020 14:50

Instrument :

MSVOA_V

ClientSampleId :

F2L60





Tot Ion: 96 Resp: 8624

Ion Ratio Lower Upper

96 100

61 145.3 102.4 190.2

98 64.3 44.4 82.5

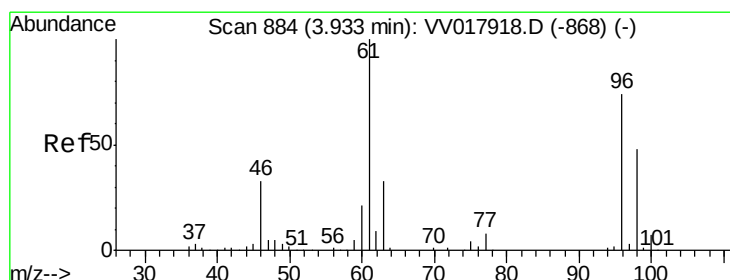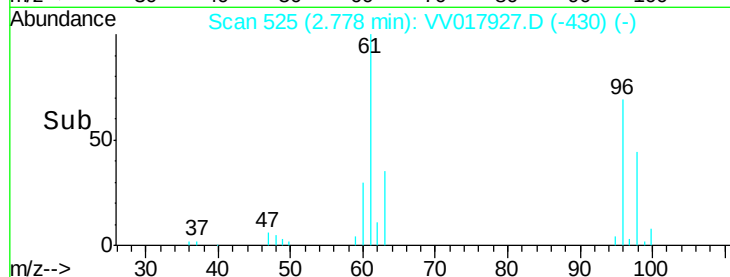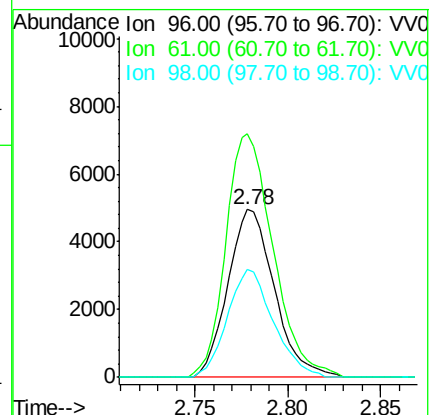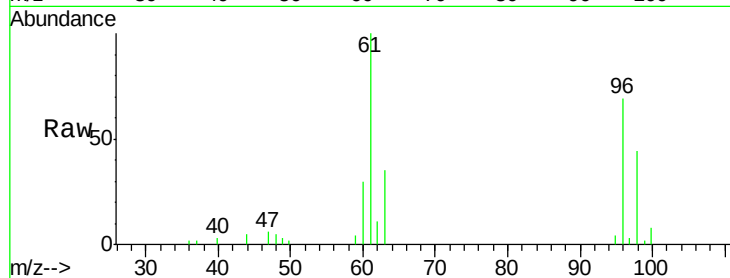

#20

cis-1,2-Dichloroethene

Concen: 388.706 ug/L

RT: 3.94 min Scan# 885

Delta R.T. 0.00 min

Lab File: VV017927.D

Acq: 12 Aug 2020 14:50




Tgt Ion: 96 Resp: 751167


Ion Ratio Lower Upper

96 100

61 136.3 95.0 176.4

68 0.0 0.0 0.0

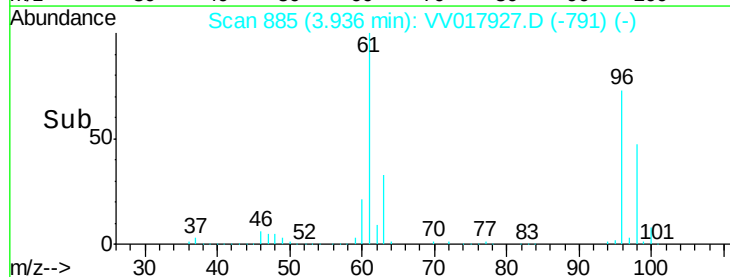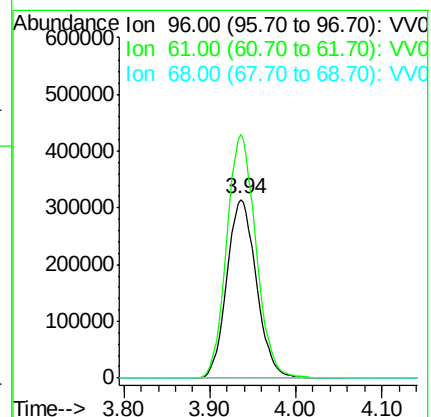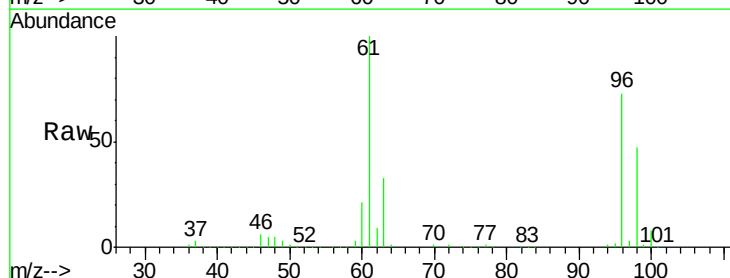

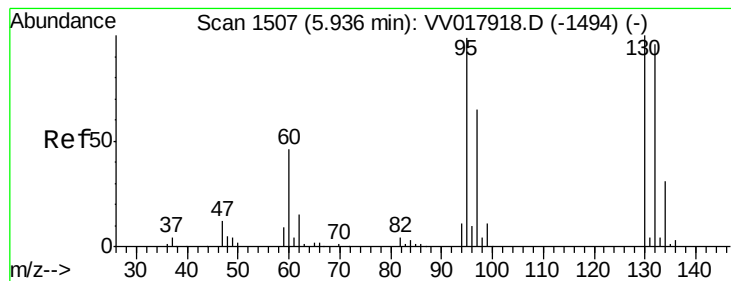

#34

Trichloroethene

Concen: 952.003 ug/L

RT: 5.94 min Scan# 1508

Delta R.T. 0.00 min

Lab File: VV017927.D

Acq: 12 Aug 2020 14:50

Instrument :

MSVOA_V

ClientSampleId :

F2L60

Tot Ion: 95 Resp: 1924285


Ion Ratio Lower Upper

95 100

97 64.6 46.0 85.4

132 95.1 65.8 122.2

130 98.8 69.2 128.6

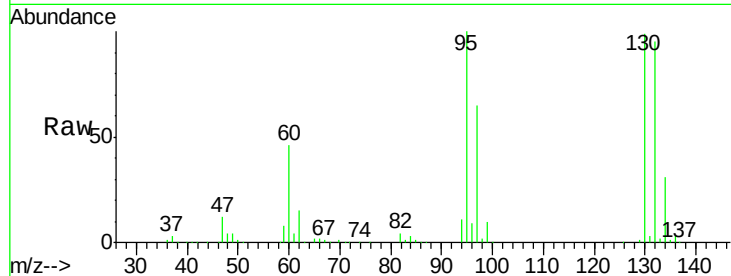




Abundance

Ion 95.00 (94.70 to 95.70): VV017918.D (-1494) (-)

Ion 97.00 (96.70 to 97.70): VV017918.D (-1494) (-)

Ion 132.00 (131.70 to 132.70): VV017918.D (-1494) (-)

Ion 130.00 (129.70 to 130.70): VV017918.D (-1494) (-)

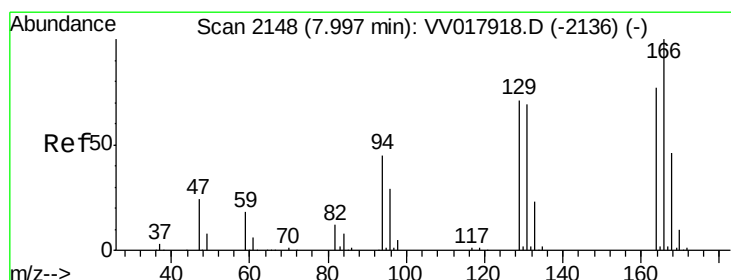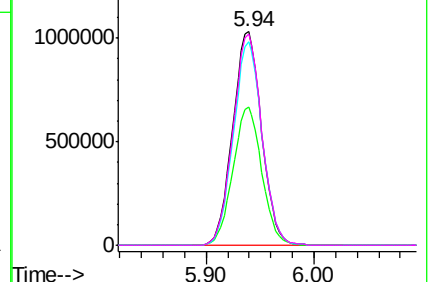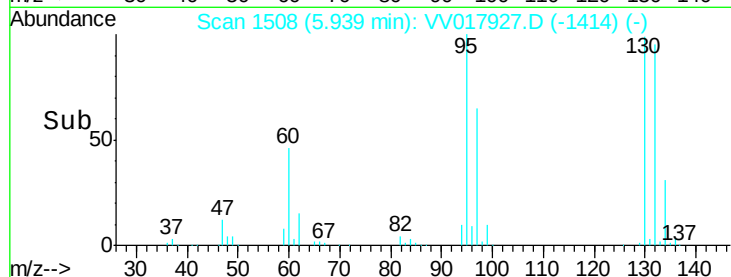

#46

Tetrachloroethene

Concen: 606.078 ug/L

RT: 8.00 min Scan# 2148

Delta R.T. 0.00 min

Lab File: VV017927.D

Acq: 12 Aug 2020 14:50

Tgt Ion: 164 Resp: 898455


Ion Ratio Lower Upper

164 100

129 94.1 64.8 120.3

131 90.0 64.5 119.9

166 126.8 88.9 165.1

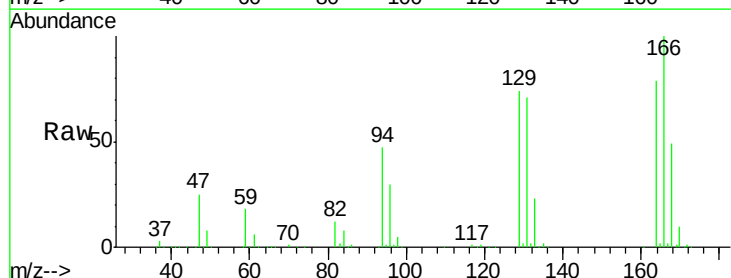

Abundance

Ion 164.00 (163.70 to 164.70): VV017918.D (-2136) (-)

Ion 129.00 (128.70 to 129.70): VV017918.D (-2136) (-)

Ion 131.00 (130.70 to 131.70): VV017918.D (-2136) (-)

Ion 166.00 (165.70 to 166.70): VV017918.D (-2136) (-)

