

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081220\
 Data File : VV017942.D
 Acq On : 12 Aug 2020 22:13
 Operator : SY/MD
 Sample : L3644-07DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2L60DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	228952	236227	15.47%	1.955%
2	1.579	144	152	165	rBV	182943	205196	13.44%	1.698%
3	2.122	311	321	348	rVB	372537	567936	37.20%	4.699%
4	2.524	436	446	458	rBV5	2402	4531	0.30%	0.037%
5	2.781	517	526	537	rBV3	2708	5006	0.33%	0.041%
6	2.865	550	552	555	rVB2	192	95	0.01%	0.001%
7	3.203	654	657	663	rBV2	84	76	0.00%	0.001%
8	3.232	663	666	668	rBV2	95	53	0.00%	0.000%
9	3.261	673	675	678	rVB2	257	105	0.01%	0.001%
10	3.537	758	761	764	rVB	213	129	0.01%	0.001%
11	3.576	771	773	777	rBV2	95	67	0.00%	0.001%
12	3.595	777	779	782	rVV	88	47	0.00%	0.000%
13	3.769	826	833	836	rBV2	137	146	0.01%	0.001%
14	3.936	866	885	917	rBV3	209871	685300	44.88%	5.670%
15	4.376	1005	1022	1051	rBV	242164	595178	38.98%	4.924%
16	4.553	1075	1077	1078	rBV2	297	122	0.01%	0.001%
17	4.675	1113	1115	1117	rBV	145	88	0.01%	0.001%
18	4.724	1125	1130	1133	rBV2	193	167	0.01%	0.001%
19	4.868	1172	1175	1176	rBV	166	93	0.01%	0.001%
20	4.881	1177	1179	1182	rVV2	121	84	0.01%	0.001%
21	4.961	1201	1204	1208	rVB	157	109	0.01%	0.001%
22	4.981	1208	1210	1212	rVB	151	42	0.00%	0.000%
23	5.003	1212	1217	1220	rBV2	116	114	0.01%	0.001%
24	5.071	1220	1238	1268	rBV2	601614	1526875	100.00%	12.633%
25	5.389	1333	1337	1340	rBV2	295	285	0.02%	0.002%
26	5.421	1344	1347	1349	rVB2	153	91	0.01%	0.001%
27	5.457	1354	1358	1362	rVV3	201	167	0.01%	0.001%
28	5.498	1368	1371	1372	rBV	142	65	0.00%	0.001%
29	5.588	1396	1399	1403	rBV2	105	69	0.00%	0.001%
30	5.643	1403	1416	1443	rBV	214911	427564	28.00%	3.538%
31	5.939	1493	1508	1537	rBV	636804	1256502	82.29%	10.396%
32	6.093	1543	1556	1587	rVB	342842	690806	45.24%	5.716%
33	6.341	1631	1633	1638	rVB3	214	159	0.01%	0.001%
34	6.367	1638	1641	1643	rBV	54	26	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081220\
 Data File : VV017942.D
 Acq On : 12 Aug 2020 22:13
 Operator : SY/MD
 Sample : L3644-07DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2L60DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

35	6.379	1643	1645	1648	rBV	221	137	0.01%	0.001%
36	6.396	1648	1650	1655	rVB2	197	130	0.01%	0.001%
37	6.437	1655	1663	1666	rBV2	278	442	0.03%	0.004%
38	6.469	1670	1673	1674	rBV	181	91	0.01%	0.001%
39	6.563	1696	1702	1704	rBV2	202	163	0.01%	0.001%
40	6.608	1714	1716	1718	rVB	143	36	0.00%	0.000%
41	6.682	1737	1739	1740	rBV	146	44	0.00%	0.000%
42	6.723	1750	1752	1753	rBV	41	20	0.00%	0.000%
43	6.823	1781	1783	1787	rVB	244	90	0.01%	0.001%
44	6.846	1787	1790	1791	rBV	171	82	0.01%	0.001%
45	6.945	1817	1821	1823	rBV	164	101	0.01%	0.001%
46	7.006	1829	1840	1875	rBV	176294	318140	20.84%	2.632%
47	7.164	1886	1889	1891	rBV2	336	149	0.01%	0.001%
48	7.267	1919	1921	1922	rBV	147	49	0.00%	0.000%
49	7.338	1931	1943	1967	rBV	710185	1209733	79.23%	10.009%
50	7.643	2027	2038	2059	rBV	126955	216573	14.18%	1.792%
51	7.932	2126	2128	2129	rBV	98	38	0.00%	0.000%
52	7.952	2129	2134	2135	rBV2	271	171	0.01%	0.001%
53	7.997	2135	2148	2168	rVV	472304	789009	51.67%	6.528%
54	8.109	2173	2183	2223	rBV	296734	572569	37.50%	4.737%
55	8.395	2271	2272	2273	rBV	230	76	0.00%	0.001%
56	8.460	2289	2292	2294	rBV2	165	121	0.01%	0.001%
57	8.521	2308	2311	2314	rBV	129	81	0.01%	0.001%
58	8.592	2330	2333	2334	rBV	136	74	0.00%	0.001%
59	8.601	2334	2336	2341	rVB	494	270	0.02%	0.002%
60	8.624	2341	2343	2344	rBV	173	60	0.00%	0.000%
61	8.791	2393	2395	2396	rBV	128	32	0.00%	0.000%
62	8.826	2403	2406	2409	rVB	220	127	0.01%	0.001%
63	8.874	2409	2421	2442	rBV	333653	535289	35.06%	4.429%
64	9.116	2493	2496	2502	rBV2	193	161	0.01%	0.001%
65	9.174	2511	2514	2516	rBV	123	90	0.01%	0.001%
66	9.238	2532	2534	2537	rBV	119	73	0.00%	0.001%
67	9.309	2552	2556	2560	rBV2	304	276	0.02%	0.002%
68	9.444	2596	2598	2604	rBV2	243	184	0.01%	0.002%
69	9.563	2632	2635	2637	rBV	202	91	0.01%	0.001%
70	9.617	2650	2652	2653	rBV	114	26	0.00%	0.000%
71	9.752	2692	2694	2697	rVB	229	89	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081220\
 Data File : VV017942.D
 Acq On : 12 Aug 2020 22:13
 Operator : SY/MD
 Sample : L3644-07DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2L60DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

72	9.772	2697	2700	2701	rBV	115	76	0.00%	0.001%
73	9.907	2740	2742	2748	rVB2	224	128	0.01%	0.001%
74	10.238	2833	2845	2863	rBV	422639	654980	42.90%	5.419%
75	10.347	2877	2879	2882	rBV2	152	92	0.01%	0.001%
76	10.431	2903	2905	2906	rBV2	117	56	0.00%	0.000%
77	10.453	2910	2912	2916	rVB	183	93	0.01%	0.001%
78	10.498	2922	2926	2927	rBV	174	117	0.01%	0.001%
79	10.537	2936	2938	2940	rBV2	195	89	0.01%	0.001%
80	11.090	3108	3110	3112	rBV2	152	58	0.00%	0.000%
81	11.206	3144	3146	3148	rBV3	208	125	0.01%	0.001%
82	11.270	3155	3166	3188	rBV	311113	476294	31.19%	3.941%
83	11.456	3221	3224	3228	rBV3	238	161	0.01%	0.001%
84	11.646	3270	3283	3303	rBV	723744	1105329	72.39%	9.145%
85	12.411	3519	3521	3527	rVB2	318	173	0.01%	0.001%




Sum of corrected areas: 12086178

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081220\
Data File : VV017942.D
Acq On : 12 Aug 2020 22:13
Operator : SY/MD
Sample : L3644-07DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2L60DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

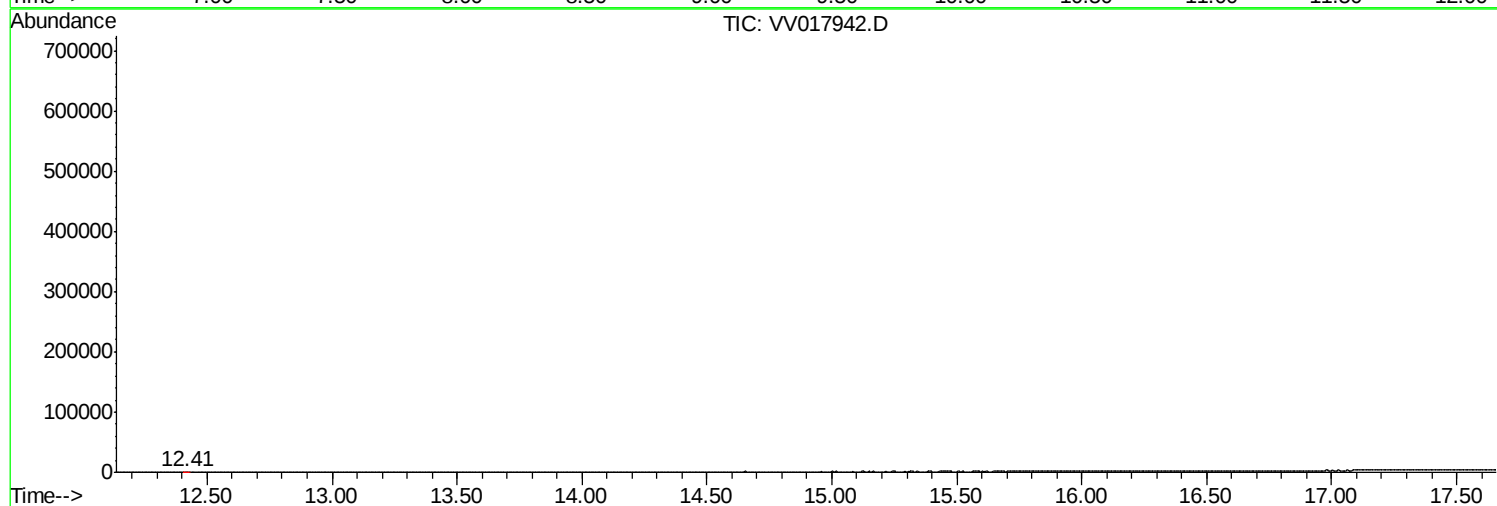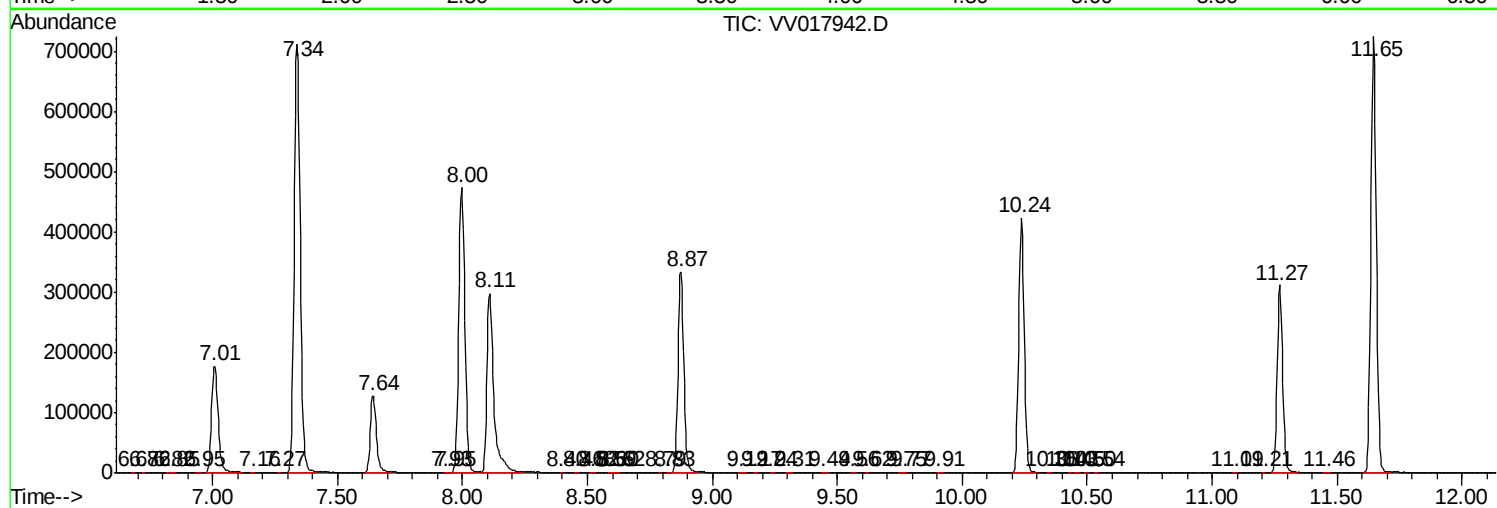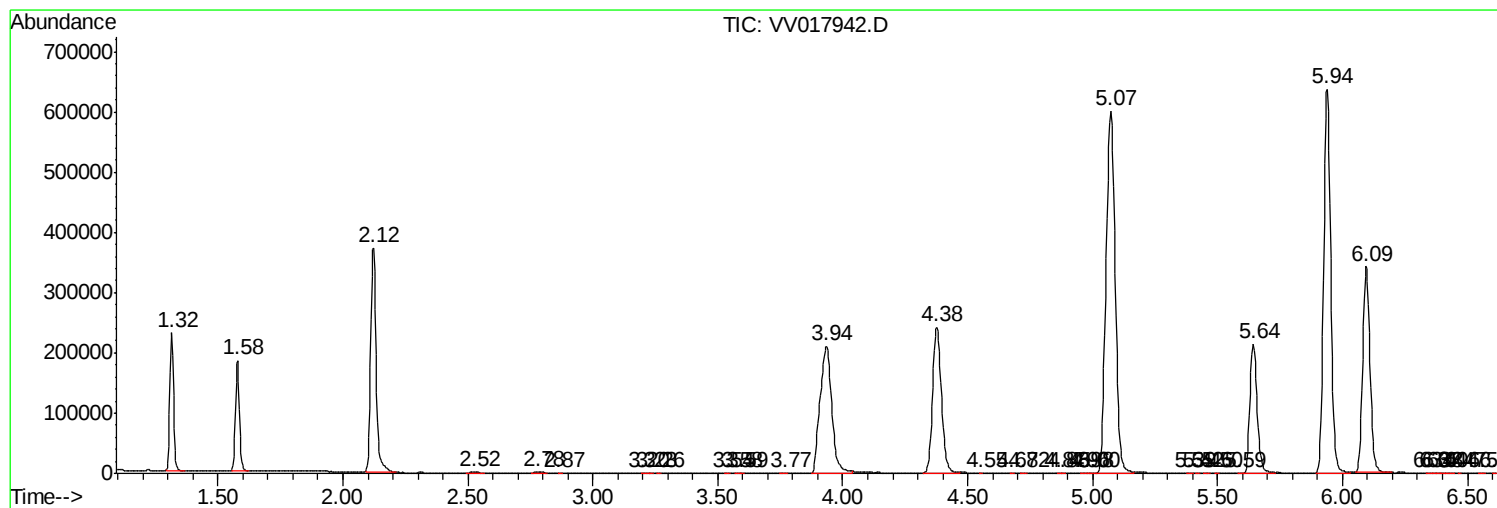

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081220\
Data File : VV017942.D
Acq On : 12 Aug 2020 22:13
Operator : SY/MD
Sample : L3644-07DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2L60DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081220\
Data File : VV017942.D
Acq On : 12 Aug 2020 22:13
Operator : SY/MD
Sample : L3644-07DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2L60DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc