

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081220\
 Data File : VV017949.D
 Acq On : 13 Aug 2020 00:57
 Operator : SY/MD
 Sample : L3665-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	103	rVB	8519933	8936505	100.00%	43.294%
2	1.579	145	152	167	rVB	113635	132380	1.48%	0.641%
3	2.122	311	321	345	rBV	231174	348642	3.90%	1.689%
4	2.357	387	394	397	rBV3	259	340	0.00%	0.002%
5	2.431	415	417	420	rBV2	191	126	0.00%	0.001%
6	2.524	441	446	452	rBV3	719	859	0.01%	0.004%
7	2.624	474	477	481	rVB	237	139	0.00%	0.001%
8	2.663	486	489	490	rBV2	183	104	0.00%	0.001%
9	2.778	513	525	553	rBV	324563	566950	6.34%	2.747%
10	2.997	589	593	598	rVB2	281	269	0.00%	0.001%
11	3.020	598	600	601	rBV2	112	51	0.00%	0.000%
12	3.045	606	608	610	rBV2	141	59	0.00%	0.000%
13	3.161	641	644	649	rVB3	280	288	0.00%	0.001%
14	3.200	649	656	658	rBV2	203	131	0.00%	0.001%
15	3.286	681	683	685	rBV2	149	66	0.00%	0.000%
16	3.325	694	695	697	rBV2	111	52	0.00%	0.000%
17	3.409	714	721	723	rBV2	124	131	0.00%	0.001%
18	3.444	730	732	735	rBV	94	65	0.00%	0.000%
19	3.489	741	746	748	rBV	99	92	0.00%	0.000%
20	3.505	748	751	754	rVB2	222	153	0.00%	0.001%
21	3.550	762	765	768	rVB2	178	108	0.00%	0.001%
22	3.569	768	771	774	rBV	81	68	0.00%	0.000%
23	3.621	784	787	795	rBV2	107	167	0.00%	0.001%
24	3.727	819	820	824	rVB2	152	53	0.00%	0.000%
25	3.817	845	848	851	rBV	79	70	0.00%	0.000%
26	3.839	851	855	859	rBV	318	326	0.00%	0.002%
27	3.936	866	885	918	rBV	1715273	4198621	46.98%	20.341%
28	4.376	1007	1022	1051	rVB	151262	381137	4.26%	1.846%
29	4.592	1085	1089	1090	rBV	107	89	0.00%	0.000%
30	4.627	1097	1100	1103	rVB2	219	147	0.00%	0.001%
31	4.650	1104	1107	1111	rBV2	309	248	0.00%	0.001%
32	4.708	1122	1125	1129	rBV2	203	205	0.00%	0.001%
33	4.814	1156	1158	1160	rBV	151	111	0.00%	0.001%
34	4.891	1179	1182	1183	rBV	196	115	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081220\
 Data File : VV017949.D
 Acq On : 13 Aug 2020 00:57
 Operator : SY/MD
 Sample : L3665-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

35	4.971	1203	1207	1208	rBV2	183	130	0.00%	0.001%
36	5.003	1215	1217	1221	rVB2	162	92	0.00%	0.000%
37	5.071	1221	1238	1271	rBV2	383393	986383	11.04%	4.779%
38	5.392	1329	1338	1357	rVB4	4910	9894	0.11%	0.048%
39	5.527	1378	1380	1383	rBV2	195	134	0.00%	0.001%
40	5.560	1387	1390	1391	rBV2	117	63	0.00%	0.000%
41	5.566	1391	1392	1396	rVB2	235	121	0.00%	0.001%
42	5.640	1401	1415	1447	rBV	298916	600307	6.72%	2.908%
43	5.875	1486	1488	1490	rBV	170	85	0.00%	0.000%
44	5.929	1494	1505	1514	rBV3	13353	27969	0.31%	0.135%
45	6.093	1542	1556	1587	rBV	218946	442478	4.95%	2.144%
46	6.228	1596	1598	1599	rBV	352	148	0.00%	0.001%
47	6.277	1611	1613	1615	rVB2	333	112	0.00%	0.001%
48	6.302	1618	1621	1624	rVB	202	107	0.00%	0.001%
49	6.425	1658	1659	1662	rVB	111	57	0.00%	0.000%
50	6.505	1682	1684	1688	rVB2	253	141	0.00%	0.001%
51	6.527	1688	1691	1693	rBV	77	54	0.00%	0.000%
52	6.550	1693	1698	1700	rVV2	74	63	0.00%	0.000%
53	6.572	1700	1705	1707	rVV	99	122	0.00%	0.001%
54	6.675	1733	1737	1739	rBV	169	123	0.00%	0.001%
55	6.871	1791	1798	1808	rBV3	298	378	0.00%	0.002%
56	6.965	1825	1827	1830	rBV	103	74	0.00%	0.000%
57	7.010	1830	1841	1864	rBV	108473	195314	2.19%	0.946%
58	7.129	1874	1878	1881	rBV2	402	280	0.00%	0.001%
59	7.164	1887	1889	1891	rBV	176	84	0.00%	0.000%
60	7.183	1892	1895	1896	rBV2	264	115	0.00%	0.001%
61	7.251	1912	1916	1918	rBV2	185	144	0.00%	0.001%
62	7.286	1925	1927	1929	rBV2	167	92	0.00%	0.000%
63	7.338	1930	1943	1963	rBV	440616	751342	8.41%	3.640%
64	7.643	2028	2038	2059	rBV	77984	133368	1.49%	0.646%
65	7.797	2083	2086	2088	rBV2	84	50	0.00%	0.000%
66	7.849	2099	2102	2105	rBV	174	102	0.00%	0.000%
67	7.862	2105	2106	2111	rVB2	158	75	0.00%	0.000%
68	7.897	2114	2117	2118	rBV2	96	57	0.00%	0.000%
69	7.920	2122	2124	2128	rVB3	123	74	0.00%	0.000%
70	7.942	2128	2131	2133	rBV2	150	101	0.00%	0.000%
71	8.000	2145	2149	2159	rVB5	945	950	0.01%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081220\
 Data File : VV017949.D
 Acq On : 13 Aug 2020 00:57
 Operator : SY/MD
 Sample : L3665-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4L25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis

72	8.109	2172	2183	2221	rBV	181516	350919	3.93%	1.700%
73	8.463	2291	2293	2294	rBV	190	79	0.00%	0.000%
74	8.495	2300	2303	2308	rBV	248	225	0.00%	0.001%
75	8.630	2343	2345	2347	rBV2	182	80	0.00%	0.000%
76	8.688	2360	2363	2369	rBV2	120	141	0.00%	0.001%
77	8.875	2409	2421	2447	rBV	461913	745829	8.35%	3.613%
78	9.068	2478	2481	2485	rBV3	244	187	0.00%	0.001%
79	9.096	2486	2490	2494	rVB2	197	160	0.00%	0.001%
80	9.164	2506	2511	2514	rBV3	387	367	0.00%	0.002%
81	9.254	2537	2539	2542	rBV2	80	65	0.00%	0.000%
82	9.283	2545	2548	2554	rVB2	130	134	0.00%	0.001%
83	9.383	2576	2579	2581	rBV	162	89	0.00%	0.000%
84	9.415	2587	2589	2590	rBV	218	77	0.00%	0.000%
85	9.505	2613	2617	2621	rBV	180	152	0.00%	0.001%
86	9.556	2630	2633	2634	rBV2	109	64	0.00%	0.000%
87	9.640	2654	2659	2662	rBV2	126	140	0.00%	0.001%
88	10.238	2832	2845	2868	rBV	275767	429146	4.80%	2.079%
89	10.389	2889	2892	2893	rBV	142	63	0.00%	0.000%
90	10.473	2916	2918	2919	rBV	154	83	0.00%	0.000%
91	10.566	2945	2947	2954	rBV3	194	199	0.00%	0.001%
92	10.617	2961	2963	2967	rVB	170	101	0.00%	0.000%
93	10.804	3019	3021	3022	rBV	204	76	0.00%	0.000%
94	10.945	3061	3065	3071	rBV2	256	203	0.00%	0.001%
95	11.122	3115	3120	3127	rBV2	204	302	0.00%	0.001%
96	11.270	3155	3166	3192	rBV	446052	688096	7.70%	3.334%
97	11.521	3241	3244	3246	rBV2	216	158	0.00%	0.001%
98	11.646	3271	3283	3301	rBV	458661	703664	7.87%	3.409%
99	11.958	3376	3380	3387	rBV2	294	360	0.00%	0.002%
100	12.588	3574	3576	3581	rBV2	179	148	0.00%	0.001%


Sum of corrected areas: 20641357

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081220\
Data File : VV017949.D
Acq On : 13 Aug 2020 00:57
Operator : SY/MD
Sample : L3665-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

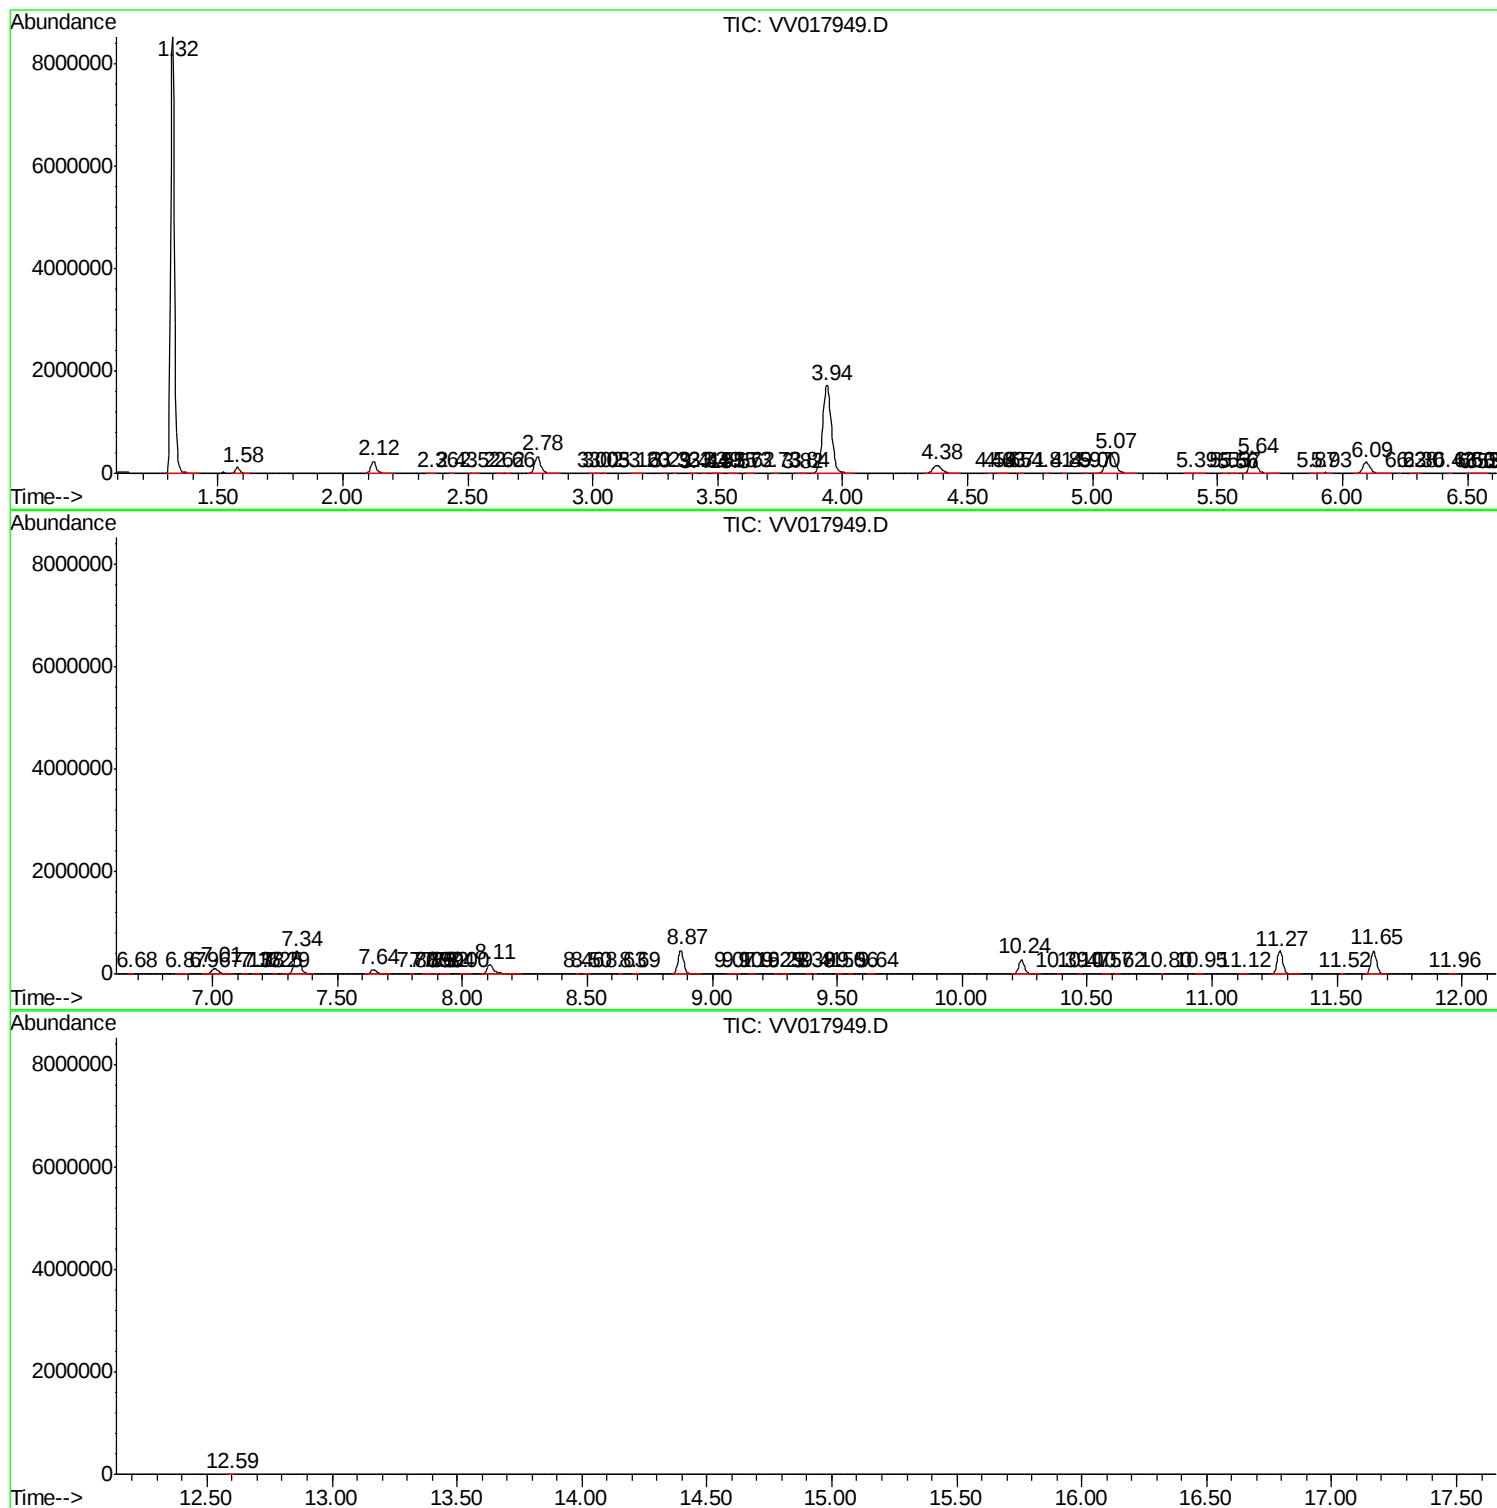

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV081220\
Data File : VV017949.D
Acq On : 13 Aug 2020 00:57
Operator : SY/MD
Sample : L3665-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV081220\
Data File : VV017949.D
Acq On : 13 Aug 2020 00:57
Operator : SY/MD
Sample : L3665-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4L25

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc