


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081220\
 Data File : VV017917.D
 Acq On : 12 Aug 2020 10:15
 Operator : SY/MD
 Sample : BFB72
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB72

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 13 05:58:58 2020

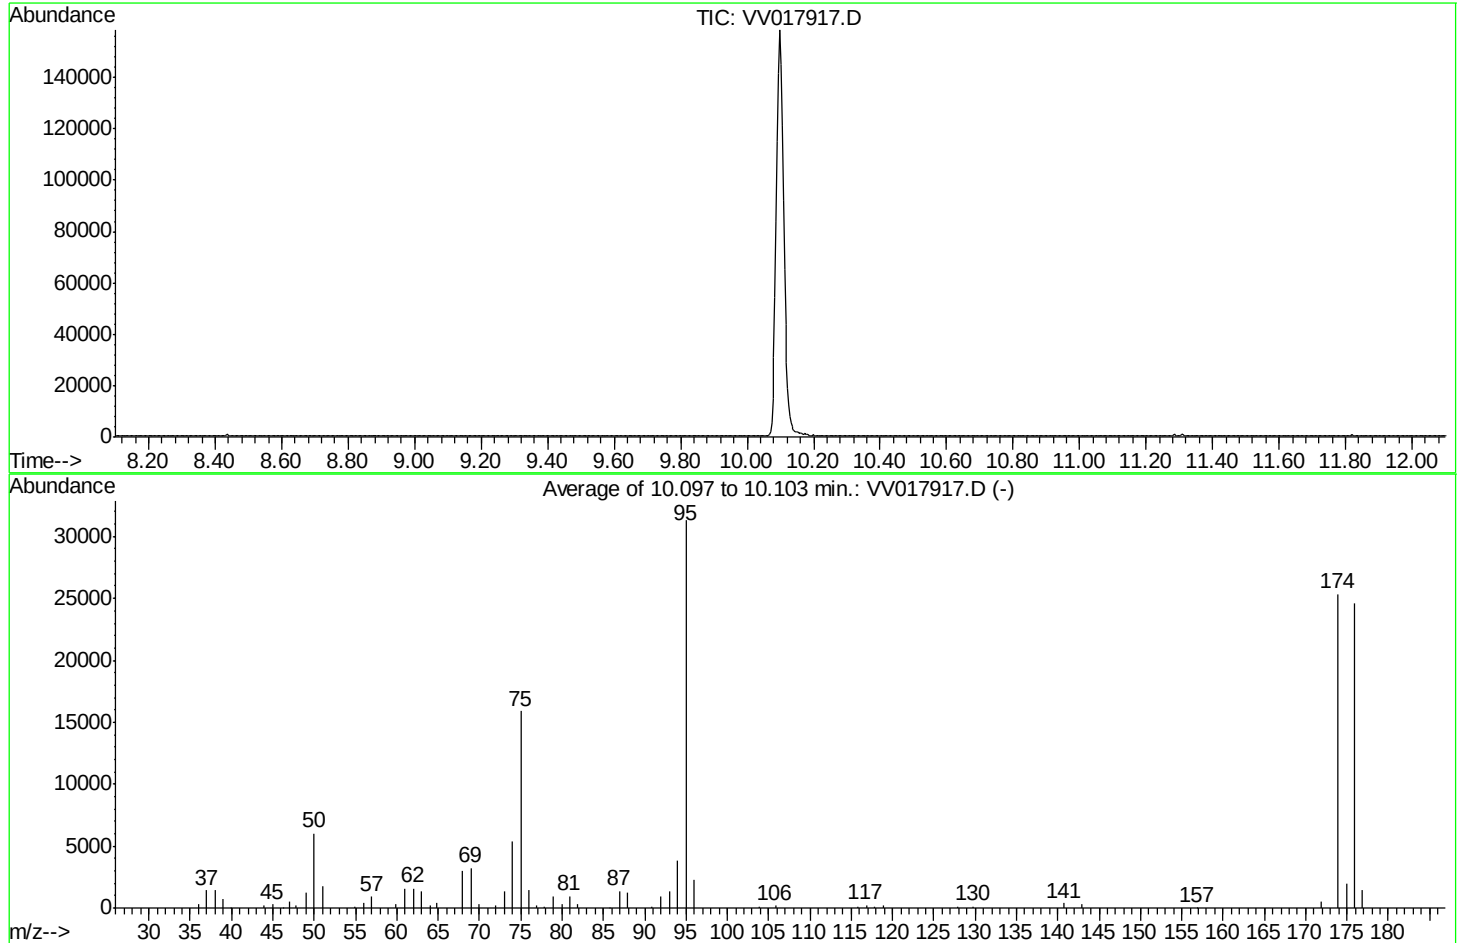

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	6037	PASS
75	95	30	80	50.7	15880	PASS
95	95	100	100	100.0	31306	PASS
96	95	5	9	7.2	2240	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.9	25333	PASS
175	174	5	9	7.6	1920	PASS
176	174	95	101	96.9	24554	PASS
177	176	5	9	6.1	1495	PASS

m/z	Abundance
35.90	288.0
37.00	1556.0
38.00	1508.0
39.00	721.0
39.90	191.0
44.00	569.0
45.00	305.0
46.20	103.0
47.00	462.0
47.80	198.0
49.00	1254.0
50.00	6274.0
51.00	1938.0
54.90	130.0
56.00	475.0
57.00	945.0
59.80	321.0
61.00	1617.0
62.00	1652.0
63.00	1384.0
64.00	219.0
64.90	468.0
68.00	2957.0
69.00	3302.0
69.90	270.0
72.00	191.0
73.00	1309.0
74.00	5737.0
75.00	16552.0
76.00	1548.0
77.00	239.0
77.90	143.0
78.90	987.0
79.90	341.0
80.90	990.0
81.80	300.0
85.80	106.0
87.00	1412.0
87.90	1288.0
90.80	119.0
92.00	1007.0
93.00	1501.0
94.00	3684.0
95.00	32096.0
96.00	2409.0
103.80	144.0
105.90	207.0
115.80	151.0
116.80	262.0
117.90	161.0
118.80	229.0
127.90	150.0
129.80	157.0
140.80	404.0
142.90	353.0
156.90	111.0
171.90	531.0
173.90	25208.0
175.00	1968.0
175.90	24640.0
176.90	1563.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	301.0
37.00	1448.0
38.00	1460.0
39.00	731.0
39.90	196.0
43.90	558.0
45.00	273.0
47.00	531.0
47.80	208.0
49.00	1283.0
50.00	6243.0
51.00	1818.0
54.90	119.0
56.00	453.0
56.90	972.0
59.90	348.0
61.00	1617.0
62.00	1654.0
63.00	1368.0
64.00	234.0
64.90	453.0
68.00	3138.0
69.00	3340.0
69.90	275.0
71.90	208.0
73.00	1335.0
74.00	5554.0
75.00	16392.0
76.00	1446.0
77.00	207.0
77.90	129.0
78.90	932.0
80.00	320.0
80.90	975.0
81.80	309.0
87.00	1433.0
87.90	1261.0
90.80	115.0
92.00	988.0
93.00	1400.0
94.00	3954.0
95.00	32440.0
96.00	2318.0
103.90	151.0
105.80	204.0
115.70	142.0
116.80	260.0
117.90	134.0
118.90	240.0
127.90	144.0
129.80	171.0
140.80	412.0
142.80	357.0
171.90	547.0
173.90	26112.0
175.00	1981.0
175.90	25376.0
176.90	1532.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	308.0
37.00	1247.0
38.00	1263.0
39.00	651.0
39.90	196.0
43.90	530.0
45.00	269.0
47.00	484.0
47.90	188.0
49.00	1198.0
50.00	5595.0
51.00	1666.0
56.00	401.0
56.90	841.0
59.90	334.0
61.00	1439.0
62.00	1466.0
63.00	1227.0
64.00	223.0
64.90	393.0
68.00	3026.0
69.00	3082.0
69.90	278.0
71.90	195.0
73.00	1336.0
74.00	4990.0
75.00	14696.0
76.00	1256.0
76.90	158.0
77.80	109.0
78.90	818.0
79.90	279.0
80.90	887.0
81.80	291.0
86.90	1307.0
88.00	1149.0
92.00	885.0
93.00	1235.0
94.00	3696.0
95.00	29384.0
96.00	1995.0
103.90	143.0
105.80	193.0
115.70	130.0
116.90	248.0
117.80	105.0
118.90	227.0
127.80	117.0
129.80	151.0
140.80	374.0
142.80	348.0
171.90	521.0
173.90	24680.0
175.00	1812.0
175.90	23648.0
176.90	1392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Scan 2790 (10.061 min): VV017917.D
BFB72

m/z	Abundance
39.90	185.0
44.00	387.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72