


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081221\
Data File : VV021773.D
Acq On : 12 Aug 2021 08:26
Operator : SY/MD
Sample : BFB204
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB204

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081121WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Aug 13 03:38:16 2021

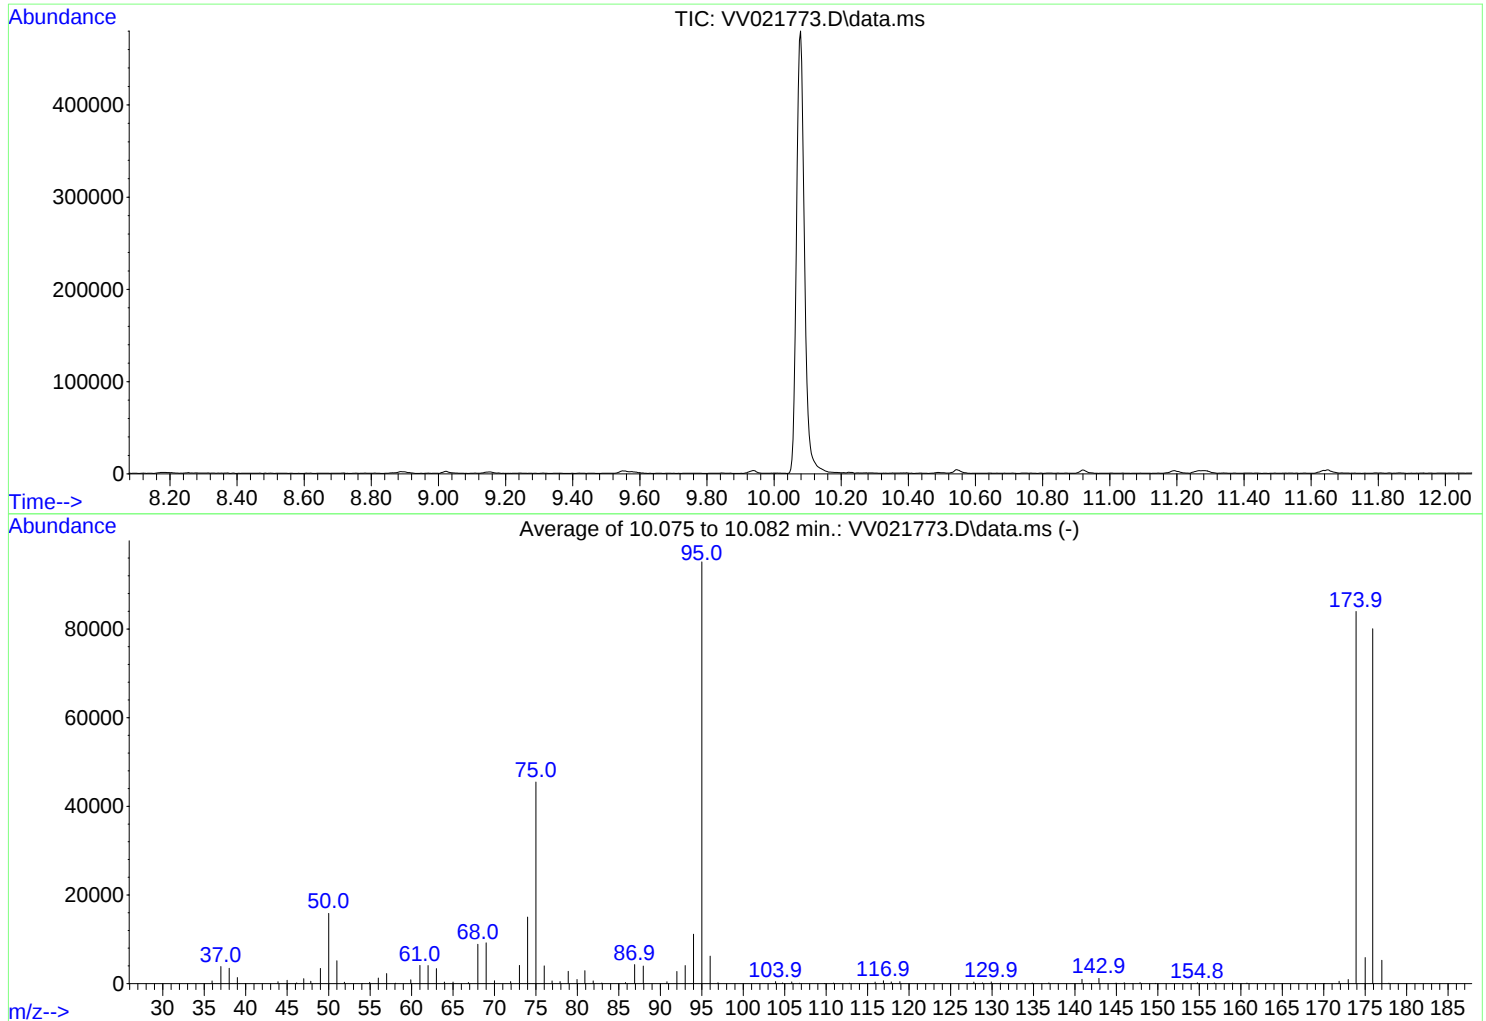

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	15853	PASS
75	95	30	80	47.8	45485	PASS
95	95	100	100	100.0	95149	PASS
96	95	5	9	6.5	6218	PASS
173	174	0.00	2	1.1	951	PASS
174	95	50	120	88.2	83952	PASS
175	174	5	9	7.0	5900	PASS
176	174	95	105	95.4	80051	PASS
177	176	5	10	6.6	5289	PASS

m/z	Abundance
36.00	638.0
37.00	3936.0
38.00	3574.0
39.00	1404.0
40.00	261.0
43.90	904.0
45.00	774.0
46.20	212.0
47.00	1114.0
47.80	585.0
49.00	3538.0
50.00	16408.0
51.00	5292.0
51.90	339.0
55.00	287.0
56.00	1290.0
57.00	2383.0
58.00	135.0
59.90	912.0
61.00	4230.0
62.00	4221.0
63.00	3548.0
63.90	398.0
65.00	391.0
66.90	260.0
68.00	9092.0
69.00	9454.0
70.00	677.0
71.90	496.0
73.00	4223.0
74.00	15391.0
75.00	46840.0
76.00	4130.0
76.90	627.0
77.90	495.0
78.90	2879.0
80.00	958.0
80.90	3008.0
81.90	629.0
82.90	141.0
85.80	260.0
86.90	4477.0
87.90	4062.0
90.80	451.0
92.00	2860.0
93.00	4231.0
94.00	11461.0
95.00	98008.0
96.00	6396.0
97.00	228.0
103.90	485.0
104.70	173.0
105.90	390.0
106.80	115.0
110.90	150.0
112.80	117.0
115.00	117.0
115.90	376.0
116.90	665.0
117.80	434.0
118.90	451.0
127.80	391.0
128.90	182.0
129.90	404.0
131.00	135.0
134.80	151.0
136.80	197.0
140.90	968.0
141.80	134.0
142.90	1243.0
144.90	153.0
146.00	205.0
147.90	249.0
149.70	120.0
154.80	206.0
156.80	146.0
159.00	152.0
160.70	143.0
170.10	102.0
171.90	551.0
172.90	978.0
173.90	86736.0
175.00	6099.0
175.90	82880.0
177.00	5511.0
177.80	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
36.00	619.0
37.00	3674.0
38.00	3341.0
39.00	1374.0
40.00	232.0
43.90	774.0
45.00	762.0
46.10	170.0
47.00	1221.0
47.90	494.0
49.00	3431.0
50.00	15025.0
51.00	4682.0
51.90	351.0
54.10	105.0
54.90	257.0
56.00	1244.0
57.00	2106.0
58.10	129.0
59.90	869.0
61.00	3847.0
62.00	3685.0
63.00	3046.0
64.00	367.0
65.00	353.0
66.80	247.0
68.00	8307.0
69.00	8742.0
70.00	585.0
71.90	451.0
73.00	3956.0
74.00	14141.0
75.00	43480.0
76.00	3759.0
77.00	562.0
77.90	433.0
78.90	2768.0
79.90	869.0
80.90	2663.0
81.90	602.0
82.90	132.0
85.80	236.0
86.90	3808.0
87.90	4001.0
90.80	397.0
92.00	2701.0
93.00	3941.0
94.00	10688.0
95.00	89712.0
96.00	5744.0
96.90	225.0
103.90	450.0
104.80	157.0
105.80	384.0
106.80	122.0
110.90	165.0
112.80	118.0
115.90	358.0
116.90	658.0
117.90	436.0
118.90	457.0
127.80	356.0
128.80	201.0
129.90	347.0
131.10	146.0
134.80	153.0
136.80	177.0
140.80	896.0
142.00	161.0
142.90	1108.0
144.90	156.0
146.00	188.0
147.70	238.0
149.70	136.0
154.70	203.0
156.80	178.0
159.00	135.0
160.70	102.0
171.80	518.0
173.00	935.0
173.90	82224.0
175.00	5631.0
175.90	78728.0
177.00	4983.0
177.90	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
39.90	217.0
43.90	423.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
35.90	612.0
37.00	3965.0
38.00	3502.0
39.00	1382.0
40.00	268.0
43.90	944.0
45.00	749.0
46.20	206.0
47.00	984.0
47.80	588.0
49.00	3337.0
50.00	16125.0
51.00	5494.0
51.90	281.0
55.00	285.0
56.00	1234.0
57.00	2387.0
58.00	103.0
59.90	870.0
61.00	4237.0
62.00	4323.0
63.00	3568.0
63.90	374.0
65.00	377.0
66.90	268.0
68.00	9223.0
69.00	9415.0
70.00	732.0
72.00	478.0
73.00	4159.0
74.00	15565.0
75.00	46136.0
76.00	4190.0
76.90	637.0
77.90	516.0
78.90	2688.0
80.00	1009.0
80.90	3108.0
81.90	635.0
83.00	125.0
85.80	226.0
86.90	4629.0
88.00	3890.0
90.80	428.0
92.00	2723.0
93.00	4022.0
94.00	11293.0
95.00	97728.0
96.00	6515.0
97.00	191.0
103.90	491.0
104.70	169.0
105.90	406.0
106.80	106.0
109.80	112.0
110.90	117.0
112.80	112.0
115.00	126.0
115.90	386.0
116.90	623.0
117.80	361.0
118.90	499.0
127.80	387.0
128.90	136.0
129.90	421.0
131.10	134.0
135.00	161.0
136.90	201.0
140.80	1031.0
141.80	123.0
142.90	1232.0
145.00	148.0
145.90	208.0
146.90	104.0
147.90	254.0
154.80	191.0
156.80	126.0
159.00	158.0
160.80	140.0
171.90	540.0
172.90	940.0
173.90	82896.0
175.00	5969.0
175.90	78544.0
177.00	5374.0
177.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204