
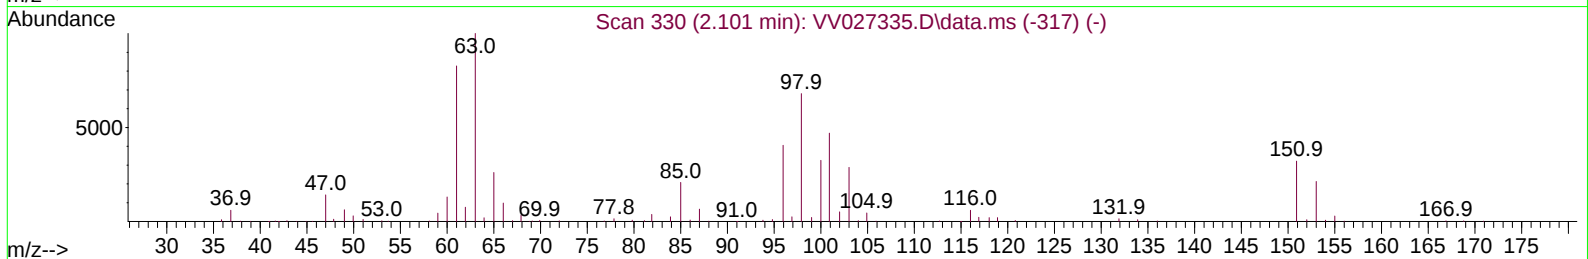
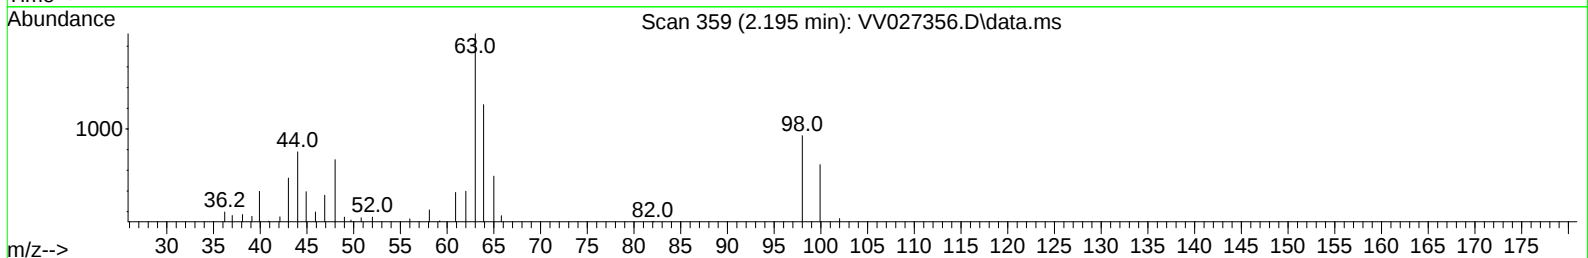


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027356.D
Acq On : 13 Aug 2022 03:28
Operator : SY/MD
Sample : N4115-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 04:20:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 02:46:03 2022
Response via : Initial Calibration

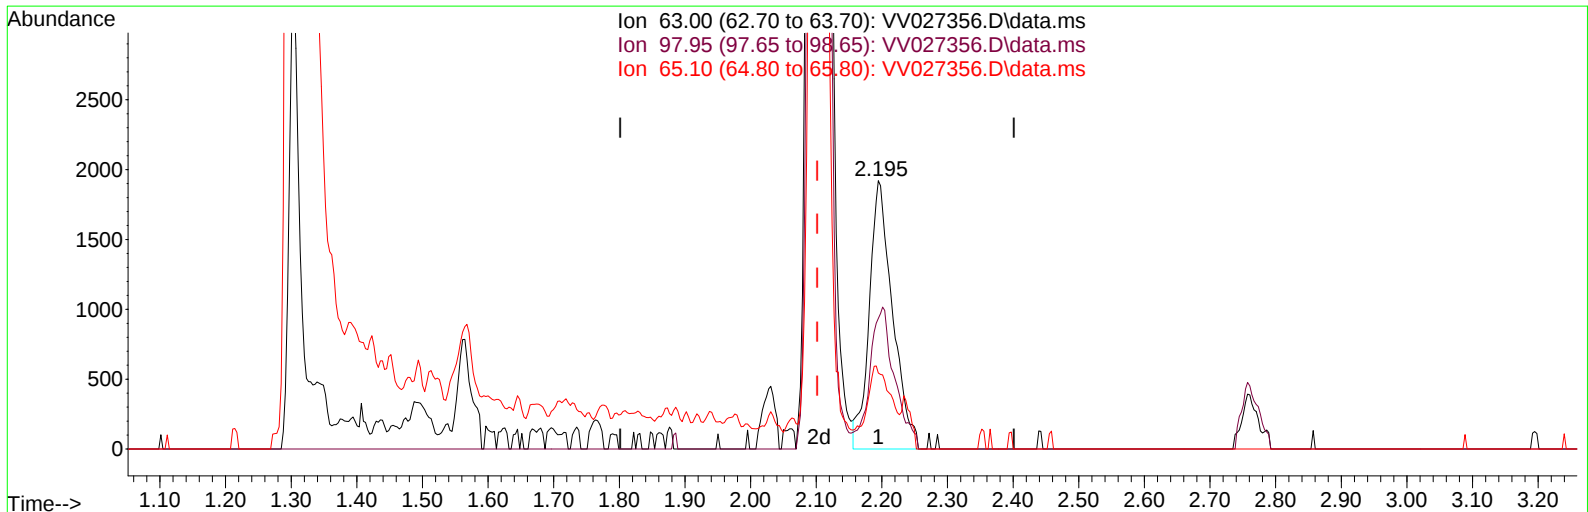

TIC: VV027356.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.195min (+ 0.093) 0.19 ug/L

response 4731

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	57.20
65.10	23.50	20.52
0.00	0.00	0.00