




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027296.D
 Acq On : 11 Aug 2022 23:22
 Operator : SY/MD
 Sample : N4161-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC14

Manual IntegrationsAPPROVED

Quant Time: Aug 12 05:46:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 02:11:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

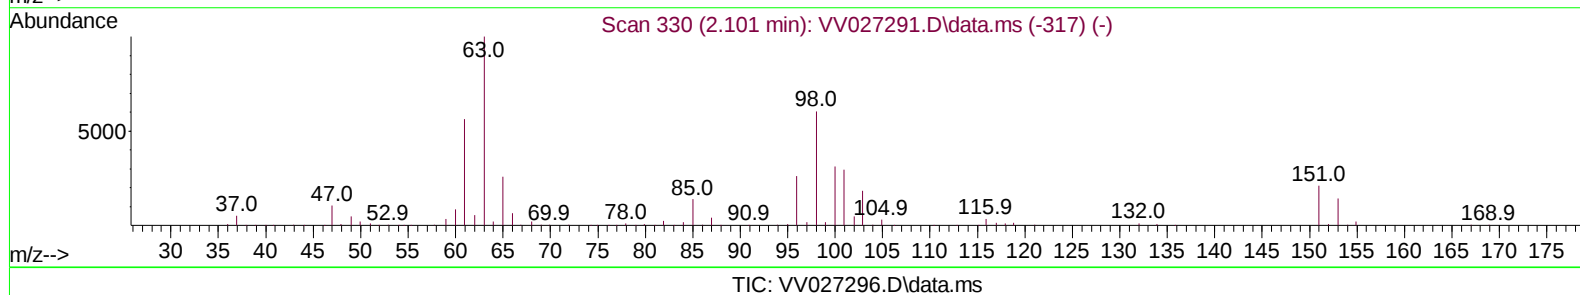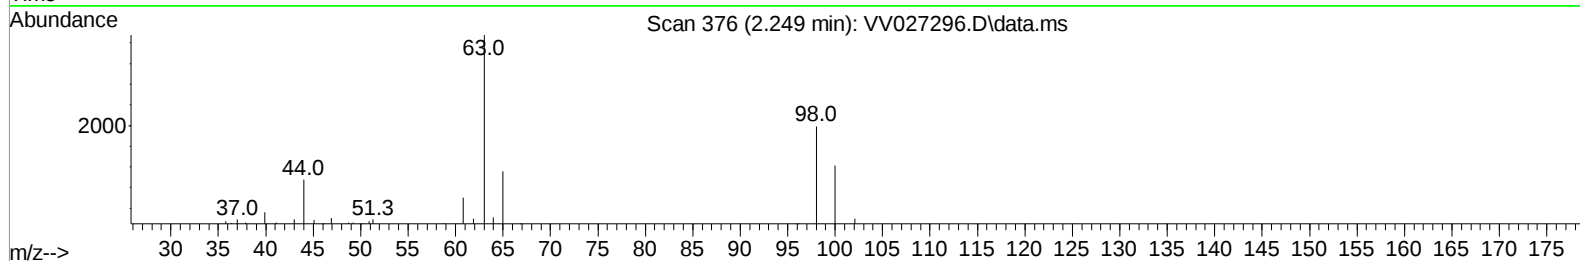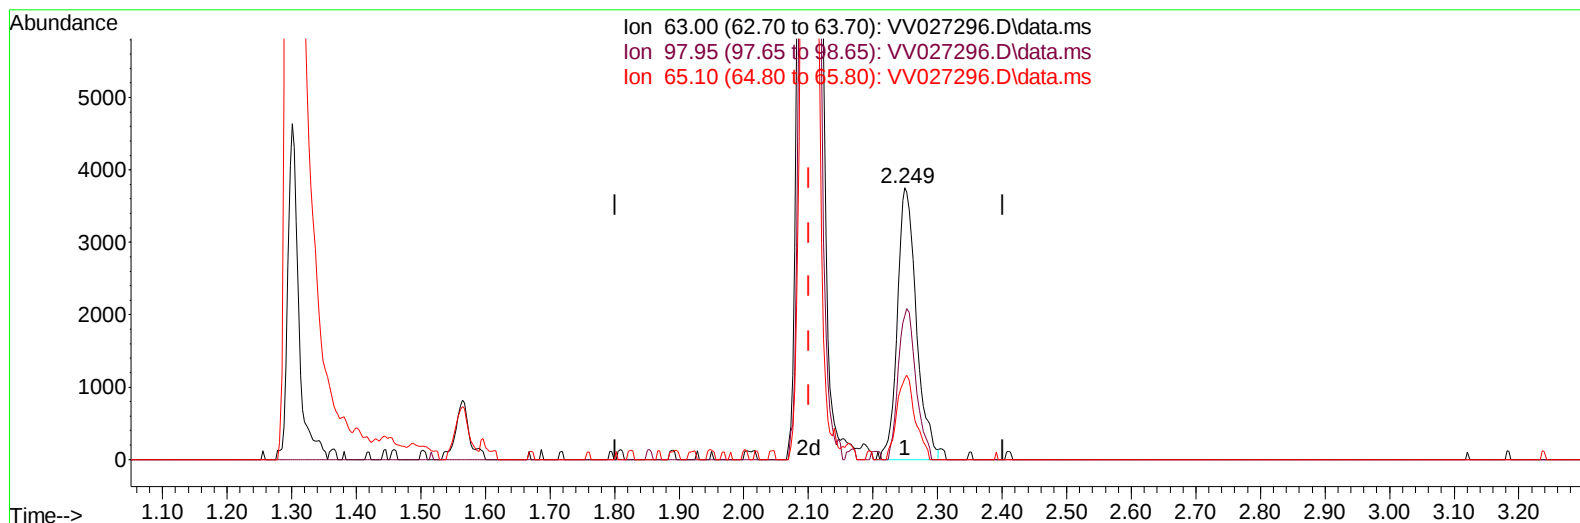

(11) 1,1-Dichloroethene-d2 (S)

2.249min (+ 0.148) 0.31 ug/L

response 7710

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	51.37
65.10	23.50	29.52
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027296.D
Acq On : 11 Aug 2022 23:22
Operator : SY/MD
Sample : N4161-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC14

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 12 05:46:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 02:11:44 2022
Response via : Initial Calibration

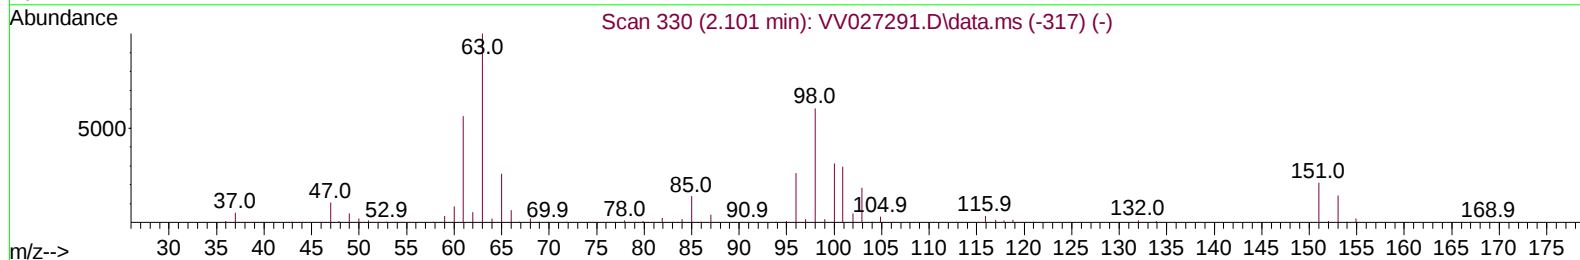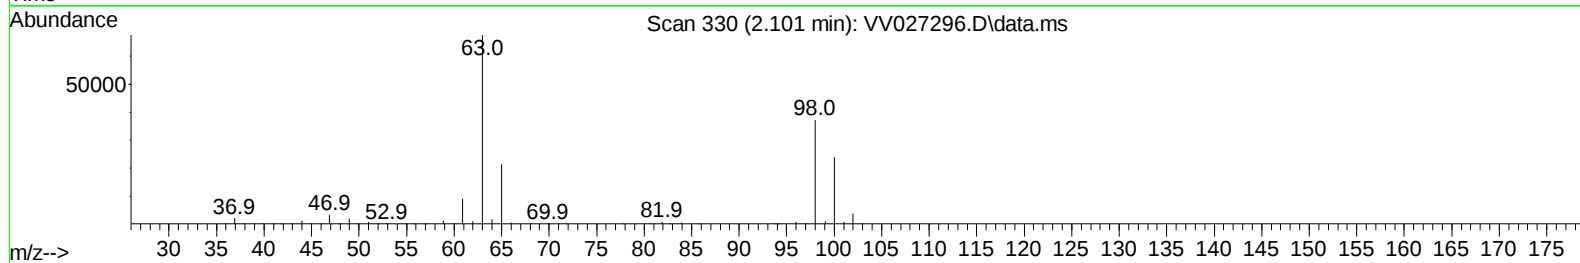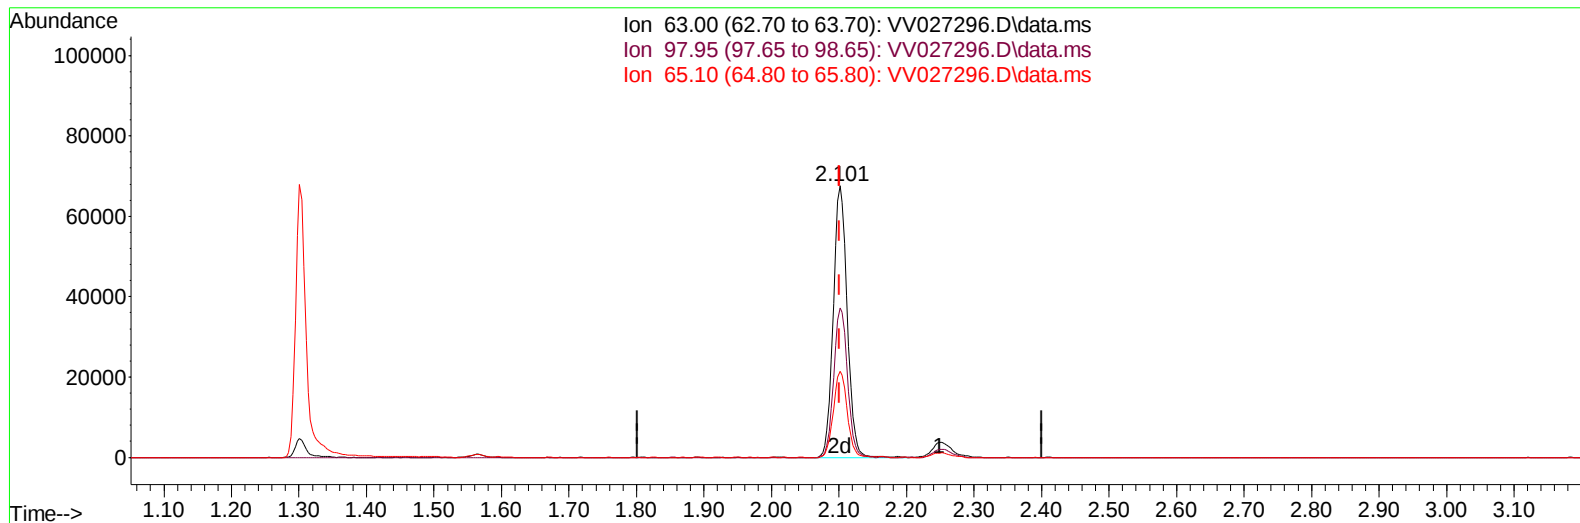

TIC: VV027296.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (+ 0.000) 3.91 ug/L m

response 96612

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	4.10#
65.10	23.50	2.36#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027296.D
 Acq On : 11 Aug 2022 23:22
 Operator : SY/MD
 Sample : N4161-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC14

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 12 05:46:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 02:11:44 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		157020	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		166726	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		69163	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		75029	5.500	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	= 110.000%		
7) Chloroethane-d5	1.561	69		53733	5.423	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	= 108.400%		
11) 1,1-Dichloroethene-d2	2.101	63		96612m	3.905	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	= 78.200%		
20) 2-Butanone-d5	3.889	46		92263	39.935	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	= 79.860%		
24) Chloroform-d	4.346	84		125536	5.018	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 100.400%		
26) 1,2-Dichloroethane-d4	5.027	65		61825	5.187	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 103.800%		
32) Benzene-d6	5.047	84		242386	4.928	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 98.600%		
36) 1,2-Dichloropropane-d6	6.066	67		77387	5.089	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	= 101.800%		
41) Toluene-d8	7.313	98		202954	4.507	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 90.200%		
43) trans-1,3-Dichloroprop...	7.625	79		24392	4.631	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	= 92.600%		
46) 2-Hexanone-d5	8.092	63		87848	43.094	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	= 86.180%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84		51003	4.636	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	= 92.800%		
66) 1,2-Dichlorobenzene-d4	11.625	152		65363	5.475	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	= 109.600%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027296.D
Acq On : 11 Aug 2022 23:22
Operator : SY/MD
Sample : N4161-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC14

Manual IntegrationsAPPROVED

Quant Time: Aug 12 05:46:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 02:11:44 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

