




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027303.D
 Acq On : 12 Aug 2022 02:17
 Operator : SY/MD
 Sample : N4162-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX9

Manual IntegrationsAPPROVED

Quant Time: Aug 12 05:48:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 02:11:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

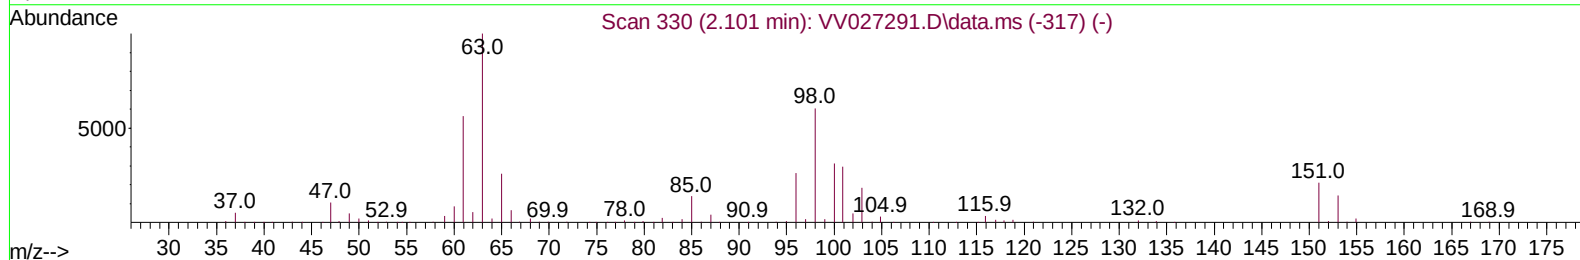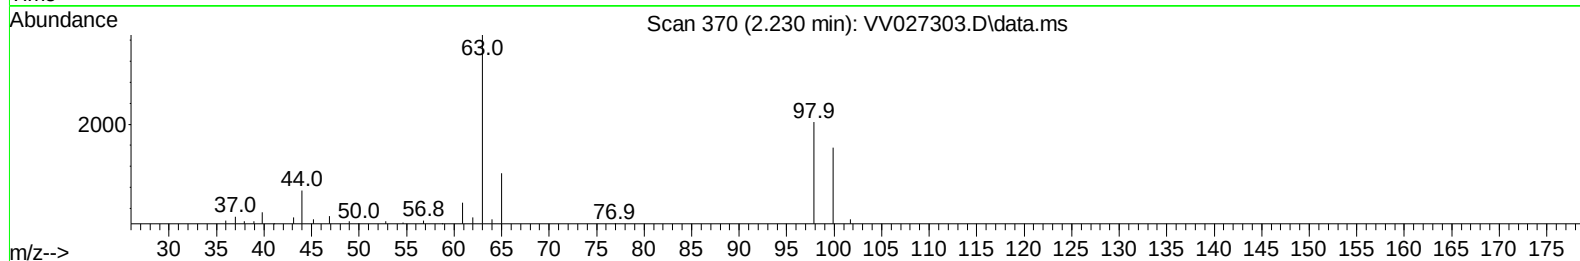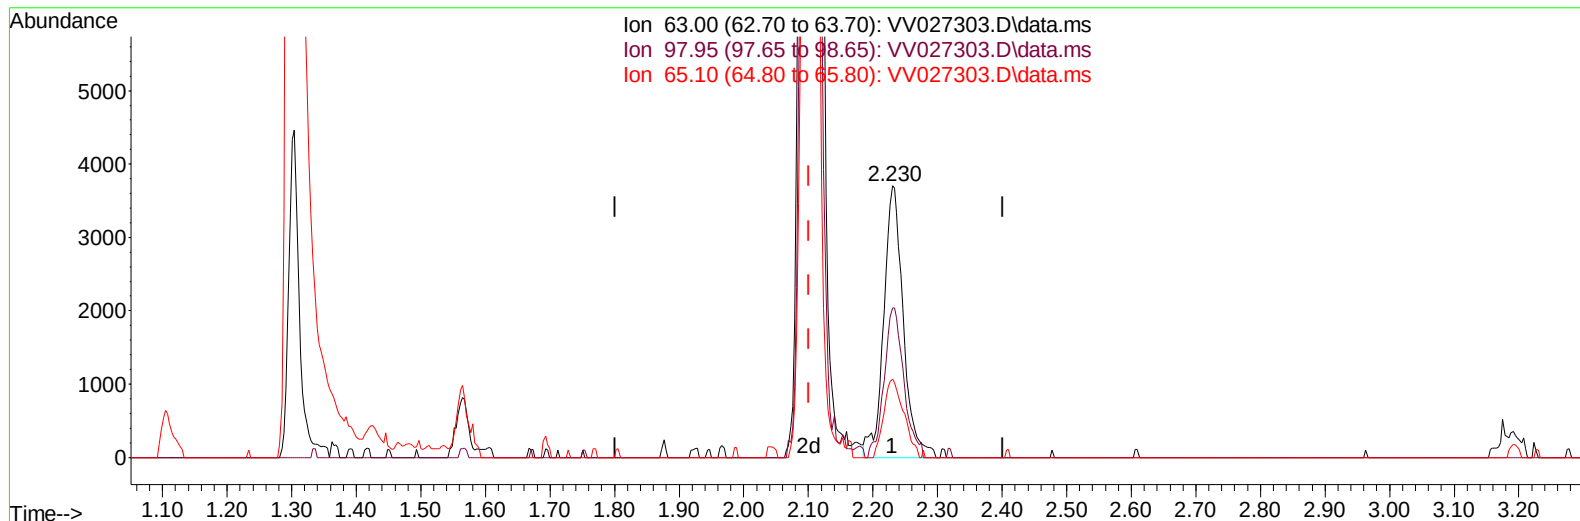

TIC: VV027303.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.230min (+ 0.129) 0.33 ug/L

response 7800

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	55.50
65.10	23.50	29.32
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027303.D
Acq On : 12 Aug 2022 02:17
Operator : SY/MD
Sample : N4162-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 12 05:48:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 02:11:44 2022
Response via : Initial Calibration

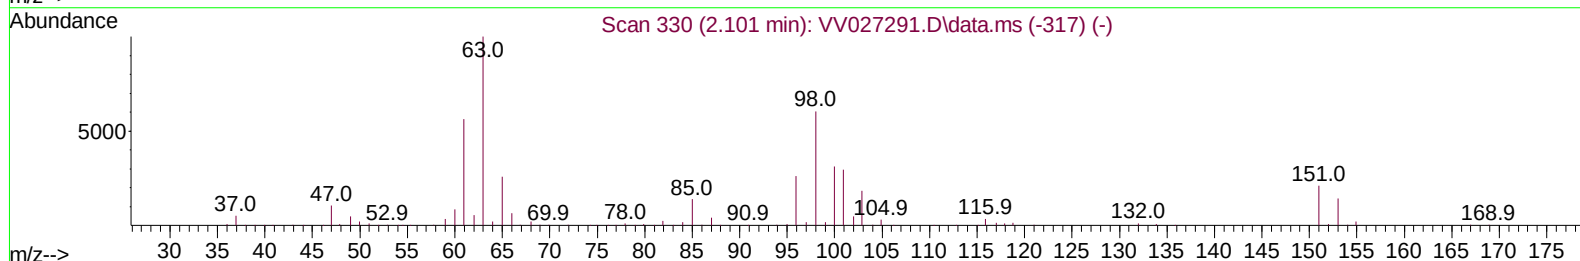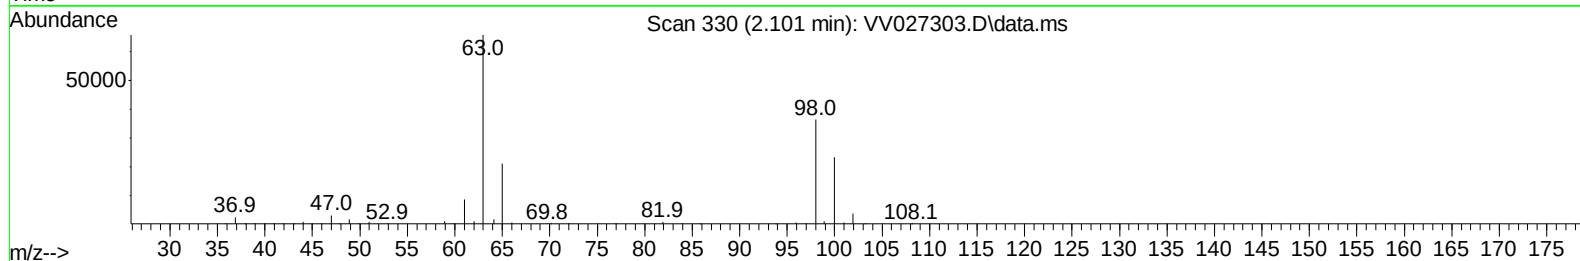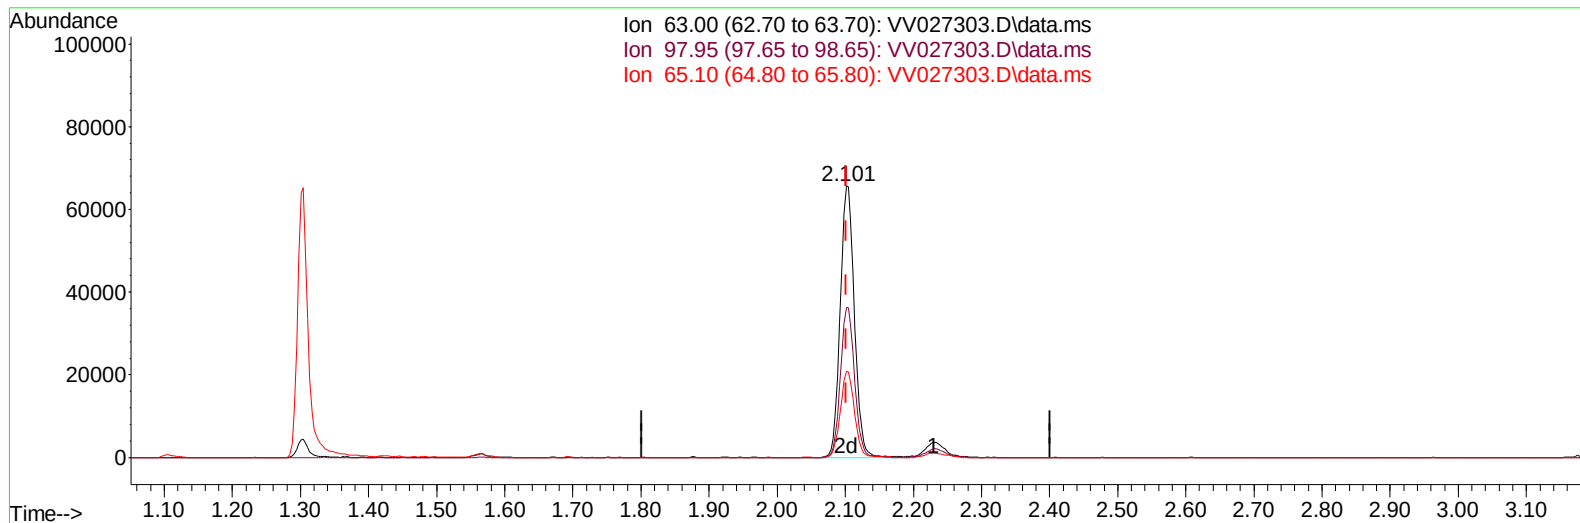

TIC: VV027303.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (+ 0.000) 3.99 ug/L m

response 94788

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	4.57#
65.10	23.50	2.41#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027303.D
 Acq On : 12 Aug 2022 02:17
 Operator : SY/MD
 Sample : N4162-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 12 05:48:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 02:11:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	150725	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	162832	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66179	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	72529	5.539	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 110.800%			
7) Chloroethane-d5	1.564	69	53043	5.577	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 111.600%			
11) 1,1-Dichloroethene-d2	2.101	63	94788m	3.991	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 79.800%			
20) 2-Butanone-d5	3.886	46	98131	44.249	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 88.500%			
24) Chloroform-d	4.346	84	123953	5.161	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 103.200%			
26) 1,2-Dichloroethane-d4	5.031	65	59317	5.184	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 103.600%			
32) Benzene-d6	5.047	84	231796	4.826	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 96.600%			
36) 1,2-Dichloropropane-d6	6.066	67	74460	5.014	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 100.200%			
41) Toluene-d8	7.313	98	192971	4.388	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 87.800%			
43) trans-1,3-Dichloroprop...	7.625	79	22107	4.297	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 86.000%			
46) 2-Hexanone-d5	8.088	63	82145	41.260	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 82.520%			
56) 1,1,2,2-Tetrachloroeth...	10.214	84	49222	4.581	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 91.600%			
66) 1,2-Dichlorobenzene-d4	11.625	152	61193	5.357	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 107.200%			
Target Compounds						
					Qvalue	
22) cis-1,2-Dichloroethene	3.912	96	8915	0.679	ug/L	99
34) Trichloroethene	5.915	95	38076	2.749	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027303.D
Acq On : 12 Aug 2022 02:17
Operator : SY/MD
Sample : N4162-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX9

Manual IntegrationsAPPROVED

Quant Time: Aug 12 05:48:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 02:11:44 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

