




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027318.D
 Acq On : 12 Aug 2022 09:20
 Operator : SY/MD
 Sample : N4162-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBZ9

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:35:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

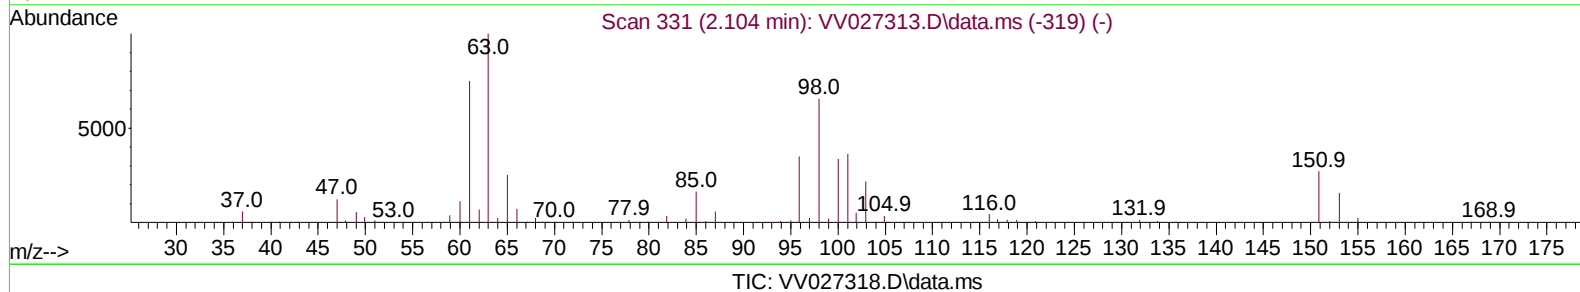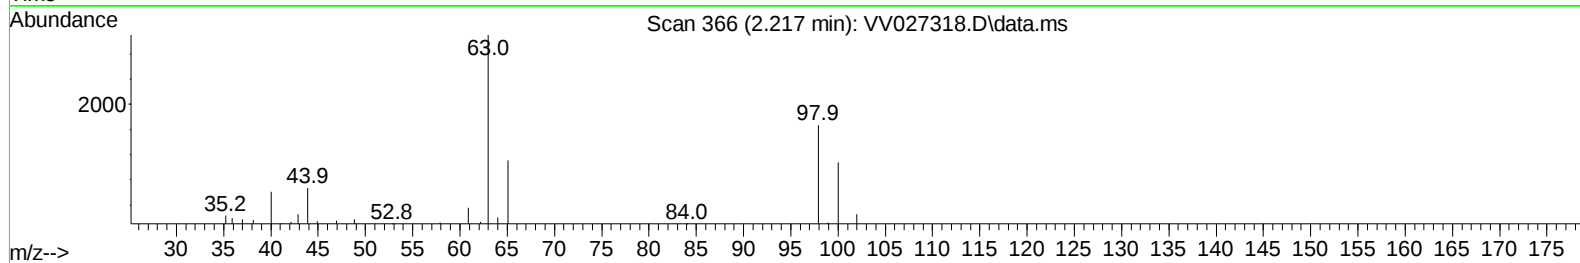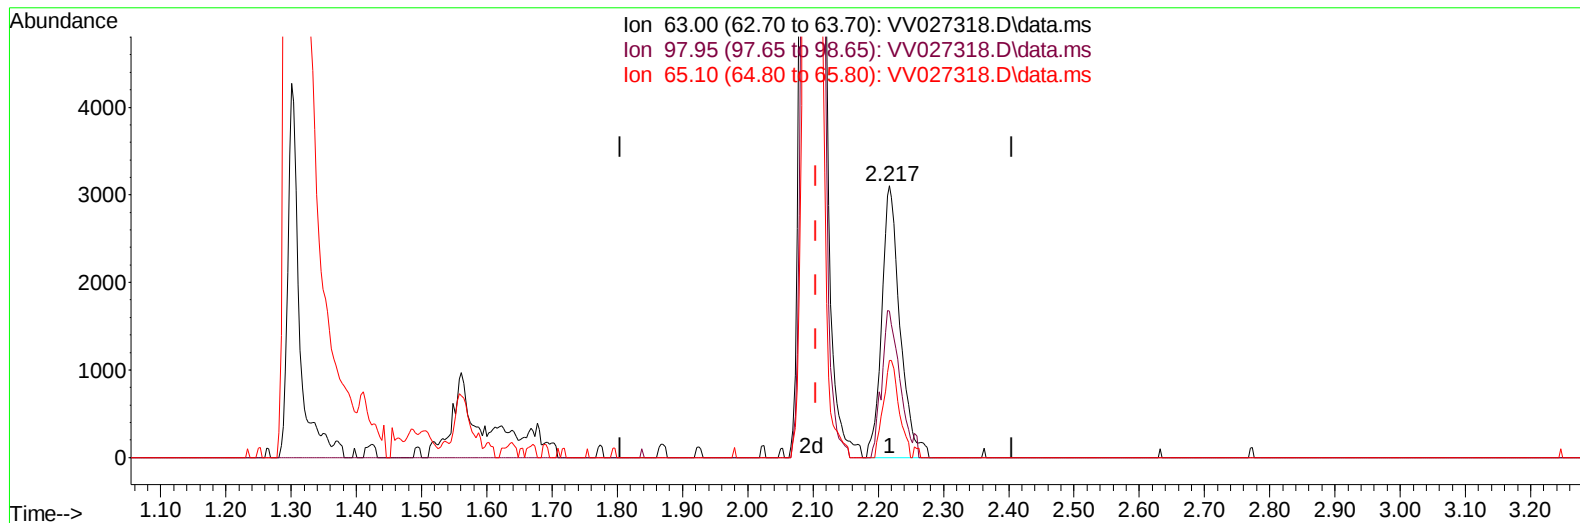

(11) 1,1-Dichloroethene-d2 (S)

2.217min (+ 0.113) 0.24 ug/L

response 6060

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	52.38
65.10	23.50	30.43
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027318.D
 Acq On : 12 Aug 2022 09:20
 Operator : SY/MD
 Sample : N4162-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBZ9

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:35:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

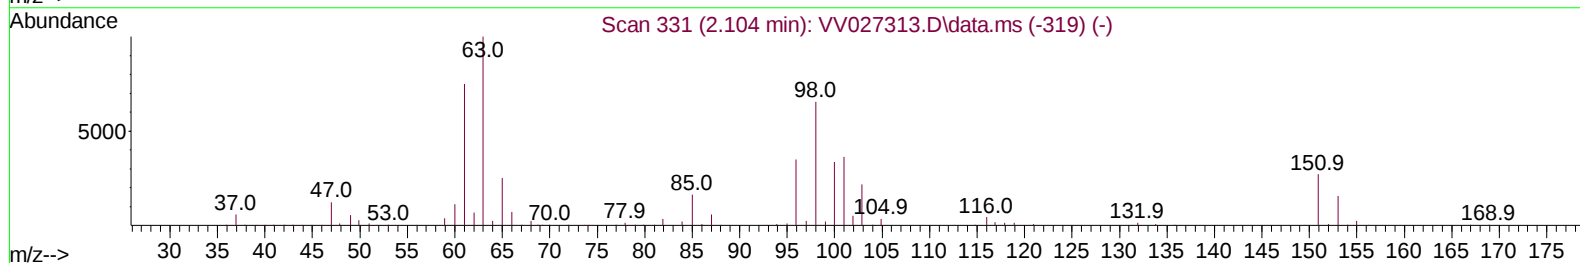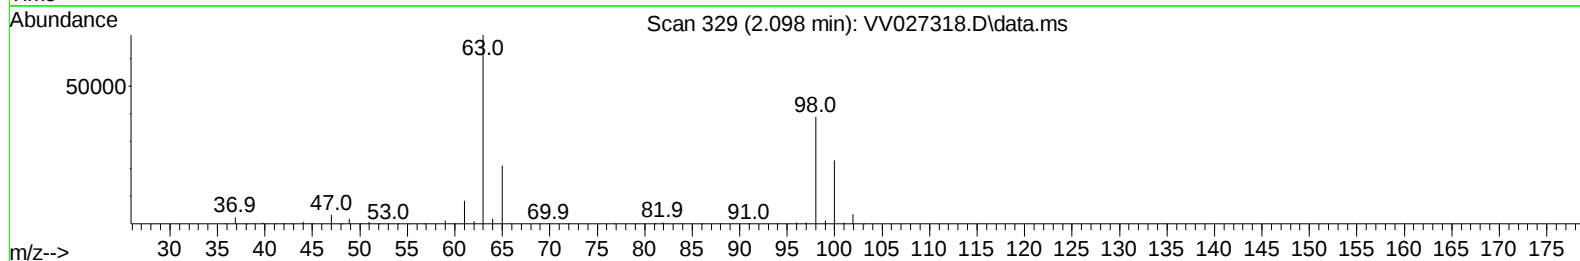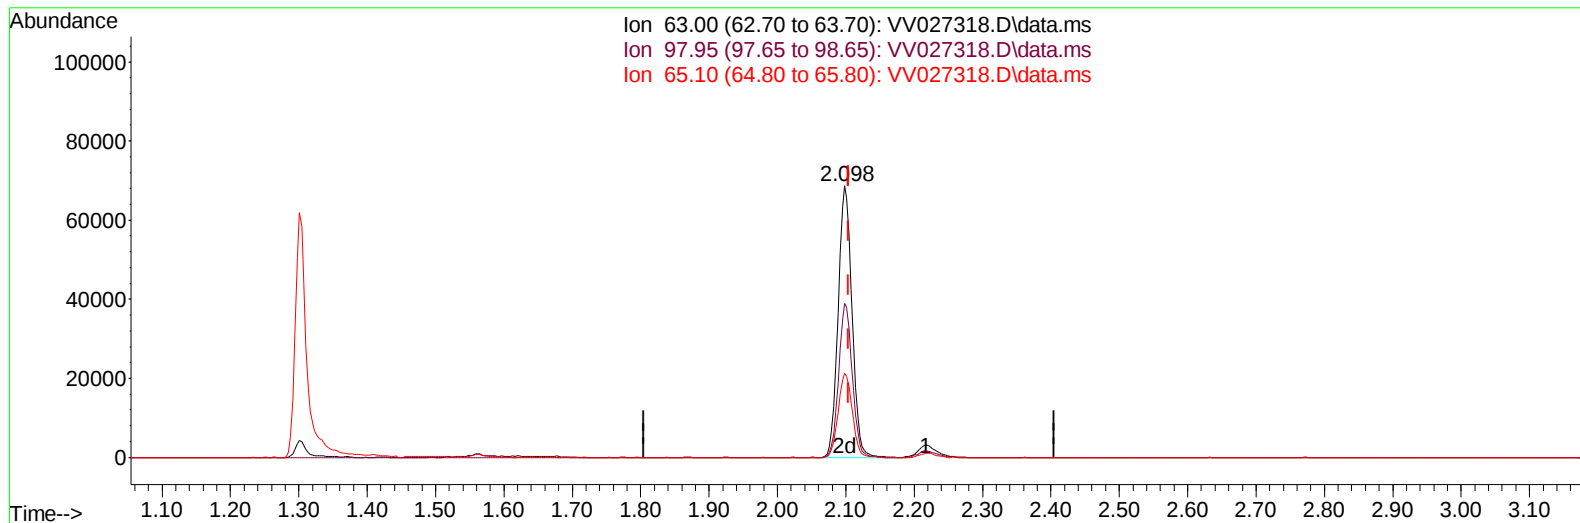

TIC: VV027318.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.098min (-0.006) 3.78 ug/L m

response 96819

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	3.28#
65.10	23.50	1.90#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027318.D
 Acq On : 12 Aug 2022 09:20
 Operator : SY/MD
 Sample : N4162-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBZ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:35:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.613	114		162677	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		170545	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		69443	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		74058	5.240	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	= 104.800%		
7) Chloroethane-d5	1.561	69		46151	4.496	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	= 90.000%		
11) 1,1-Dichloroethene-d2	2.098	63		96819m	3.777	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	= 75.600%		
20) 2-Butanone-d5	3.886	46		124561	52.040	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	= 104.080%		
24) Chloroform-d	4.343	84		127770	4.929	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 98.600%		
26) 1,2-Dichloroethane-d4	5.027	65		63508	5.143	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 102.800%		
32) Benzene-d6	5.043	84		241859	4.807	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 96.200%		
36) 1,2-Dichloropropane-d6	6.066	67		77118	4.958	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	= 99.200%		
41) Toluene-d8	7.313	98		198293	4.305	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 86.200%		
43) trans-1,3-Dichloroprop...	7.625	79		22458	4.168	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	= 83.400%		
46) 2-Hexanone-d5	8.088	63		83727	40.153	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	= 80.300%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84		50374	4.476	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	= 89.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152		64649	5.394	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	= 107.800%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027318.D
Acq On : 12 Aug 2022 09:20
Operator : SY/MD
Sample : N4162-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBZ9

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:35:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 08:00:46 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

