




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027322.D
 Acq On : 12 Aug 2022 10:59
 Operator : SY/MD
 Sample : N4164-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC09

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:36:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

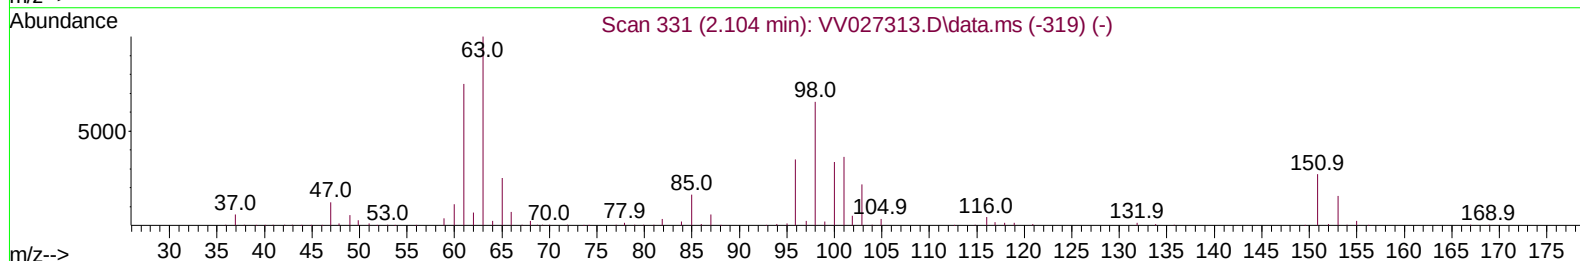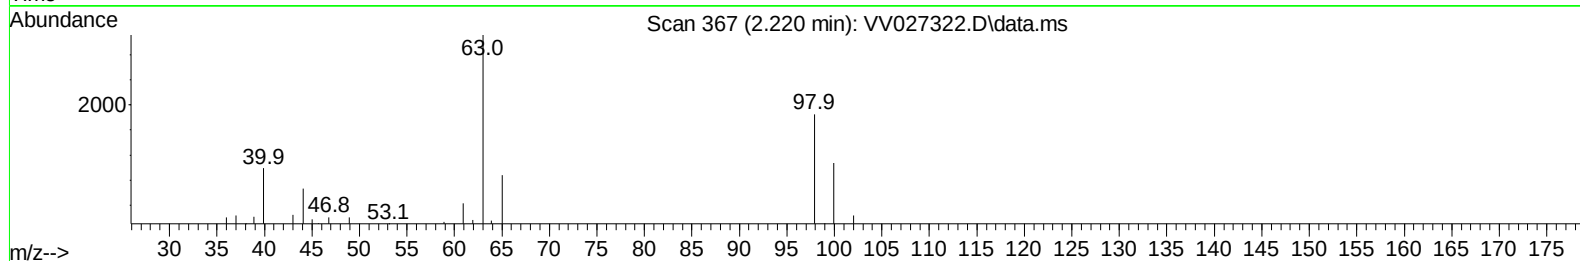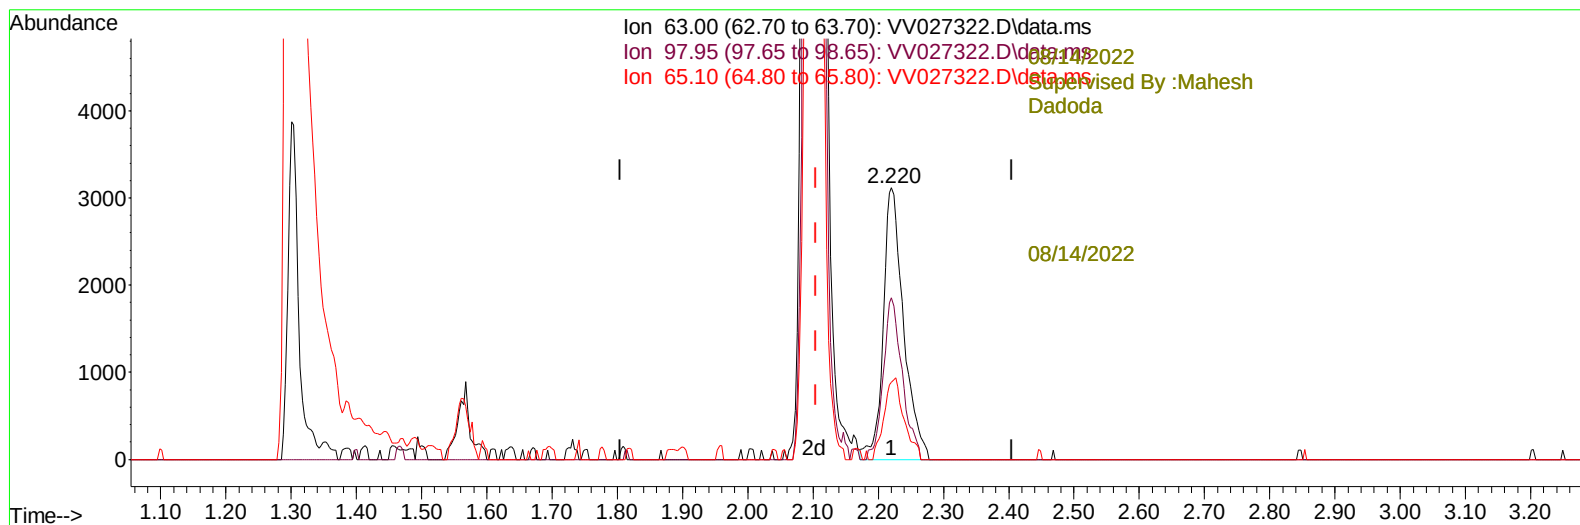

TIC: VV027322.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.220min (+ 0.116) 0.29 ug/L

response 6759

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	55.57
65.10	23.50	29.31
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027322.D
 Acq On : 12 Aug 2022 10:59
 Operator : SY/MD
 Sample : N4164-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC09

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:36:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

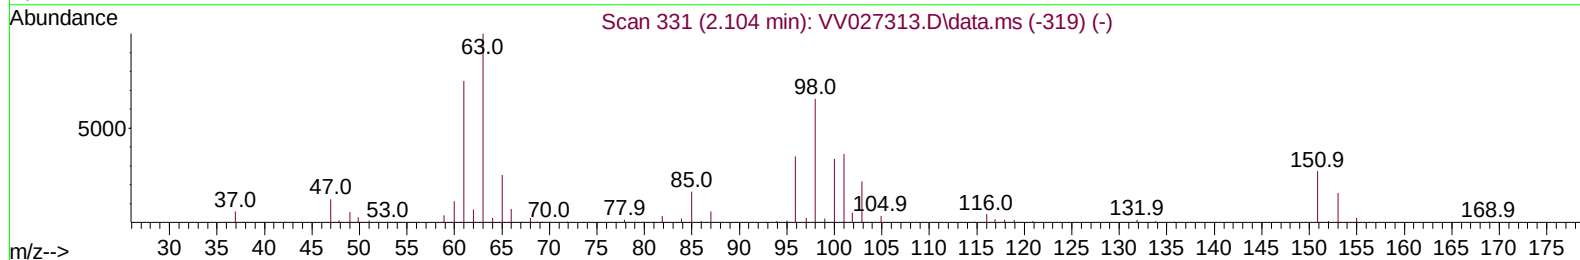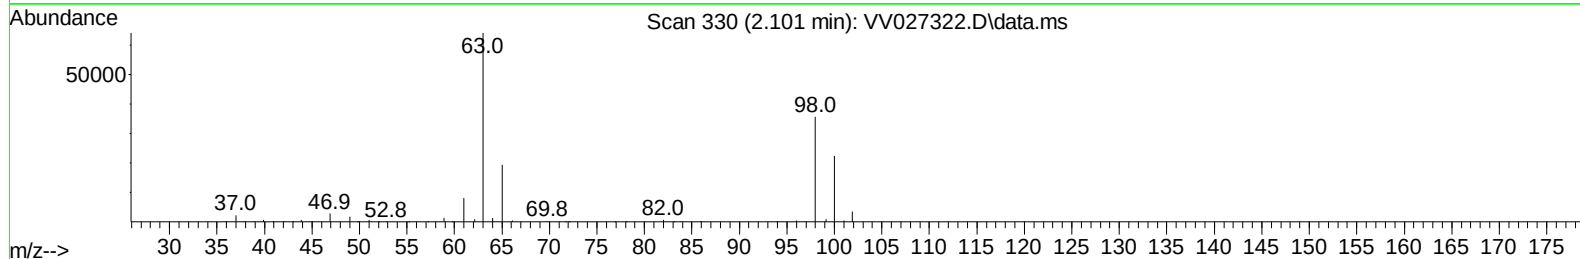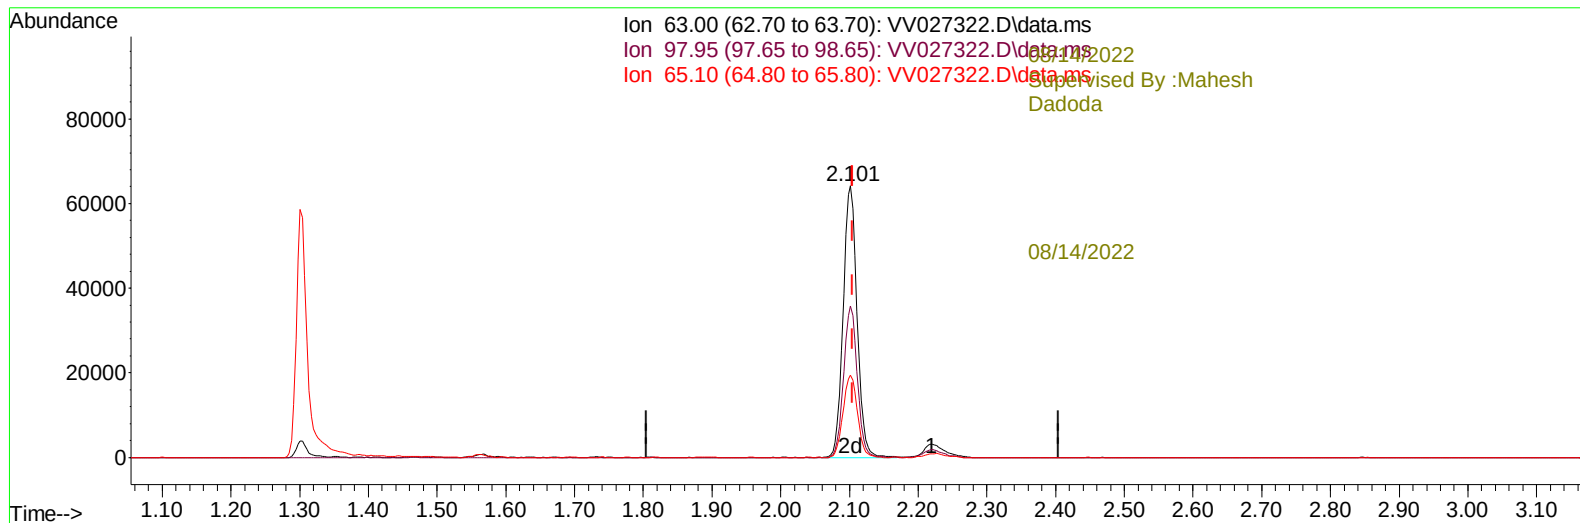

TIC: VV027322.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.003) 3.84 ug/L m

response 90344

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	4.16#
65.10	23.50	2.19#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027322.D
 Acq On : 12 Aug 2022 10:59
 Operator : SY/MD
 Sample : N4164-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC09

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:36:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----08/14/2022							
Internal Standards							
1) 1,4-Difluorobenzene	5.613	114		149289	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		161775	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		65077	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		67507	5.205	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130		Recovery	=	104.000%	
7) Chloroethane-d5	1.561	69		47646	5.058	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130		Recovery	=	101.200%	
11) 1,1-Dichloroethene-d2	2.101	63		90344m	3.841	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125		Recovery	=	76.800%	
20) 2-Butanone-d5	3.889	46		94094	42.836	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130		Recovery	=	85.680%	
24) Chloroform-d	4.343	84		122866	5.165	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125		Recovery	=	103.400%	
26) 1,2-Dichloroethane-d4	5.031	65		60542	5.342	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130		Recovery	=	106.800%	
32) Benzene-d6	5.047	84		228081	4.779	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125		Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.066	67		76560	5.189	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140		Recovery	=	103.800%	
41) Toluene-d8	7.313	98		187133	4.283	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130		Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	7.622	79		21924	4.290	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130		Recovery	=	85.800%	
46) 2-Hexanone-d5	8.088	63		78715	39.796	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130		Recovery	=	79.600%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		47449	4.445	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120		Recovery	=	88.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152		59797	5.324	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120		Recovery	=	106.400%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027322.D
Acq On : 12 Aug 2022 10:59
Operator : SY/MD
Sample : N4164-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC09

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:36:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 08:00:46 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

