




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027323.D
 Acq On : 12 Aug 2022 11:24
 Operator : SY/MD
 Sample : N4164-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC10

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:36:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

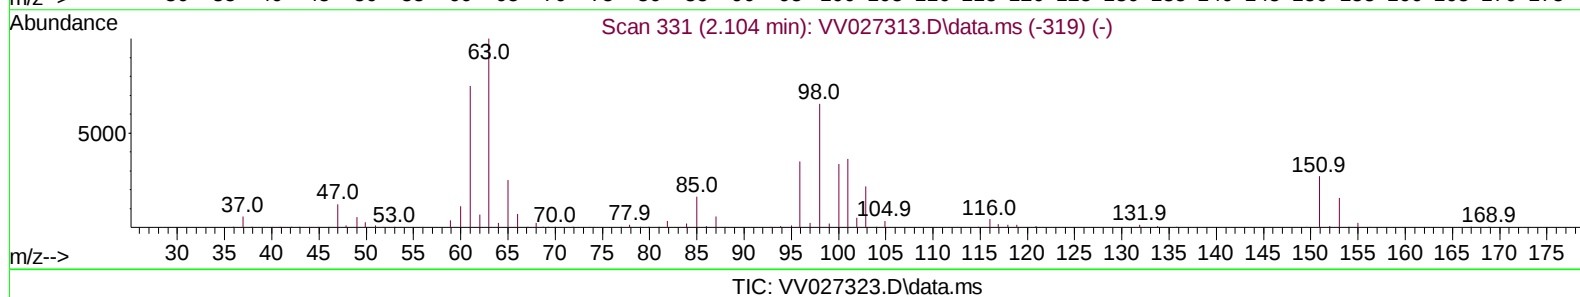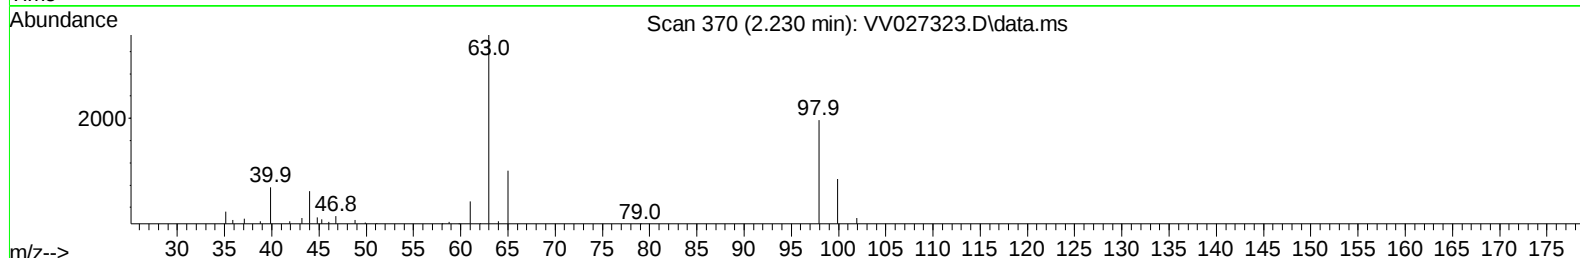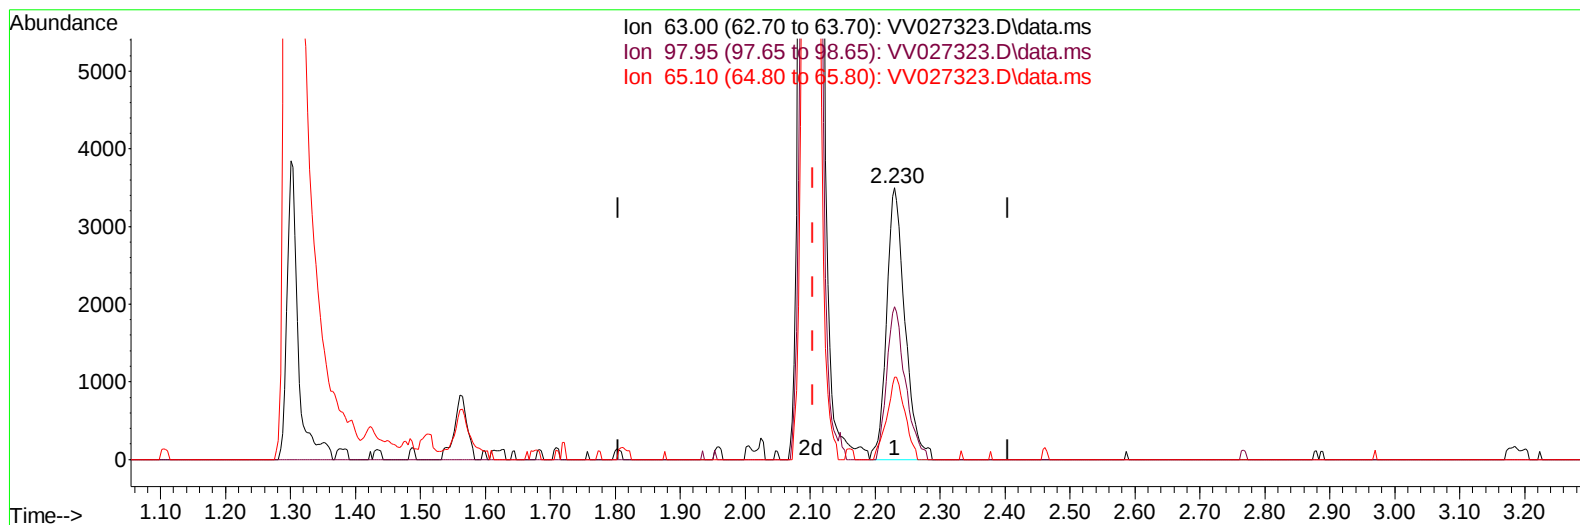

(11) 1,1-Dichloroethene-d2 (S)

2.230min (+ 0.126) 0.28 ug/L

response 6846

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	57.11
65.10	23.50	30.16
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027323.D
 Acq On : 12 Aug 2022 11:24
 Operator : SY/MD
 Sample : N4164-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC10

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:36:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

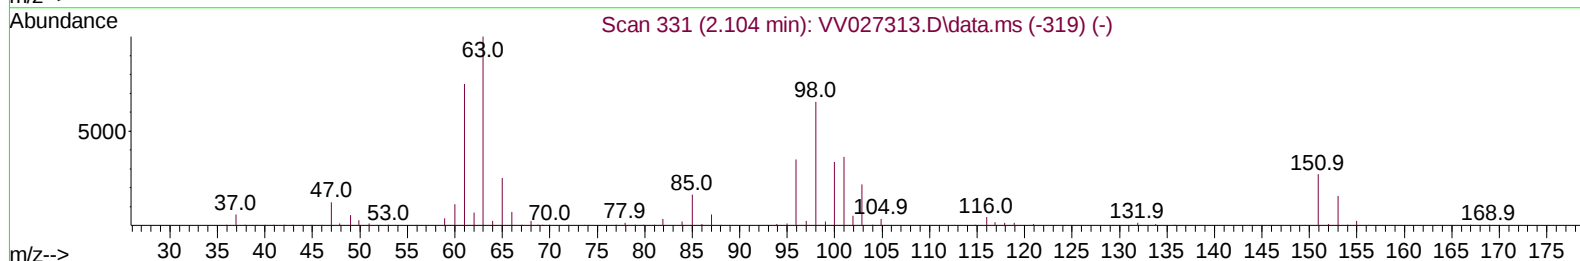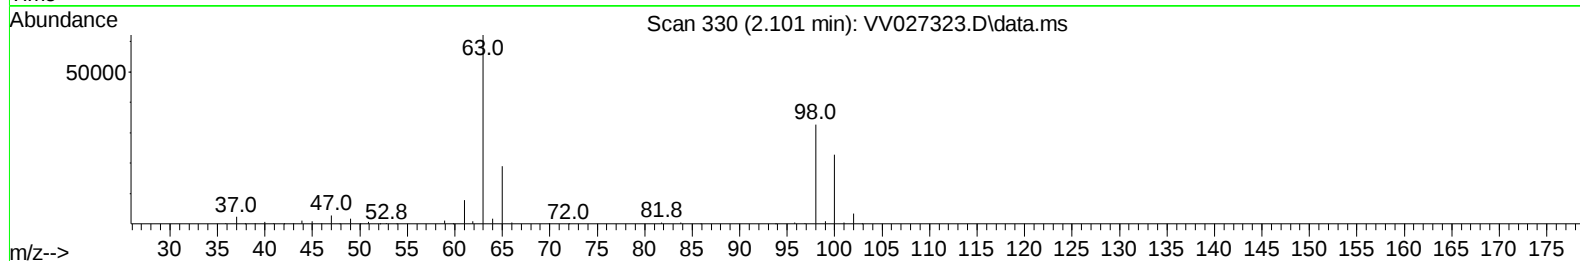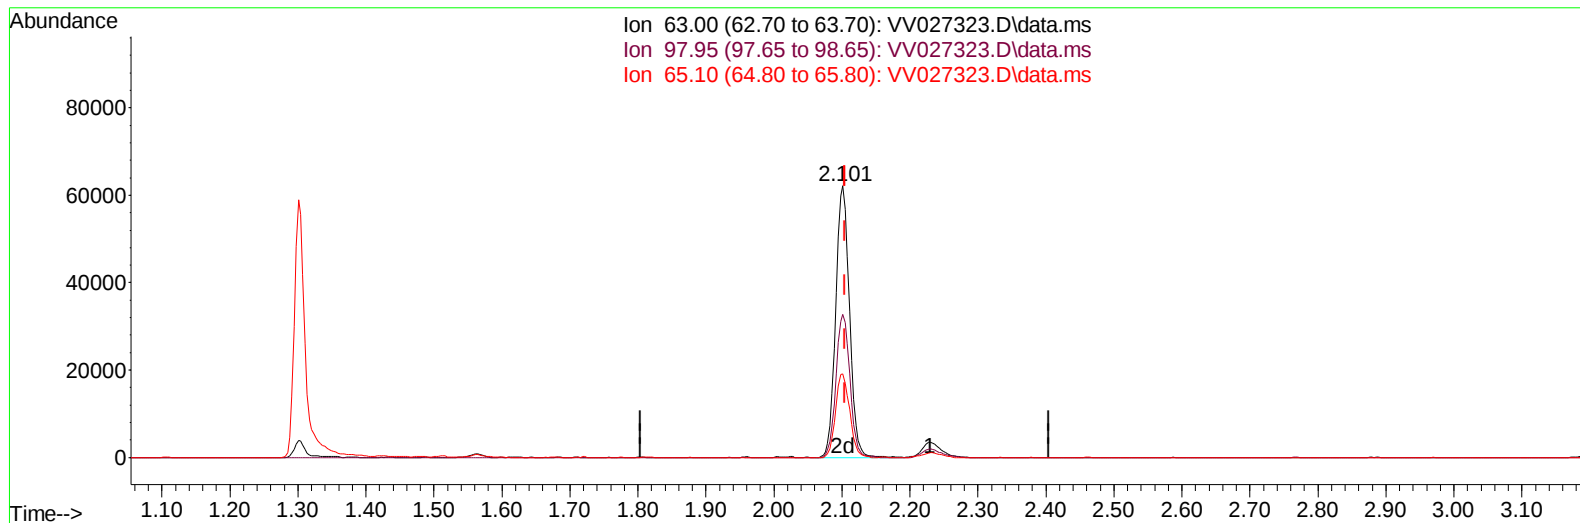

TIC: VV027323.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.003) 3.52 ug/L m

response 87456

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	4.47#
65.10	23.50	2.36#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027323.D
 Acq On : 12 Aug 2022 11:24
 Operator : SY/MD
 Sample : N4164-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC10

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:36:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.612	114		157546	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		168446	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		67575	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		67457	4.928	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.600%	
7) Chloroethane-d5	1.561	69		46406	4.668	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.400%	
11) 1,1-Dichloroethene-d2	2.101	63		87456m	3.523	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.400%	
20) 2-Butanone-d5	3.889	46		115324	49.750	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.500%	
24) Chloroform-d	4.342	84		119995	4.780	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%	
26) 1,2-Dichloroethane-d4	5.027	65		59267	4.956	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%	
32) Benzene-d6	5.047	84		222181	4.471	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%	
36) 1,2-Dichloropropane-d6	6.066	67		71903	4.680	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.600%	
41) Toluene-d8	7.313	98		182949	4.022	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.400%	
43) trans-1,3-Dichloroprop...	7.622	79		20663	3.883	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.600%	
46) 2-Hexanone-d5	8.088	63		77129	37.450	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.900%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		46420	4.176	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152		60299	5.170	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.400%	
Target Compounds							
34) Trichloroethene	5.918	95		7031	0.491	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027323.D
Acq On : 12 Aug 2022 11:24
Operator : SY/MD
Sample : N4164-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC10

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:36:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 08:00:46 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

