




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027329.D
 Acq On : 12 Aug 2022 13:54
 Operator : SY/MD
 Sample : N4145-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY148

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:37:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

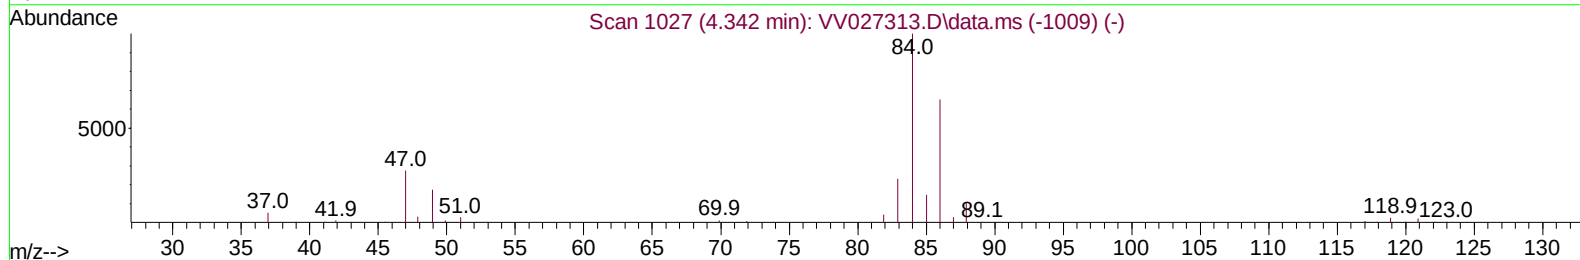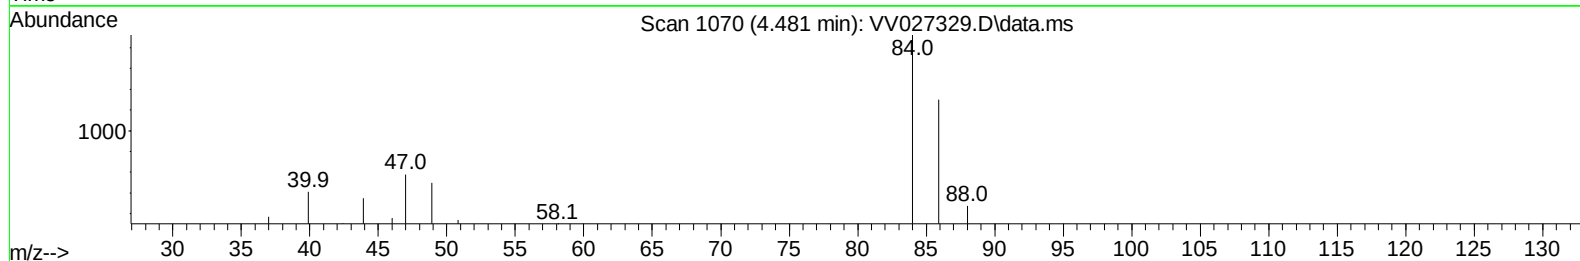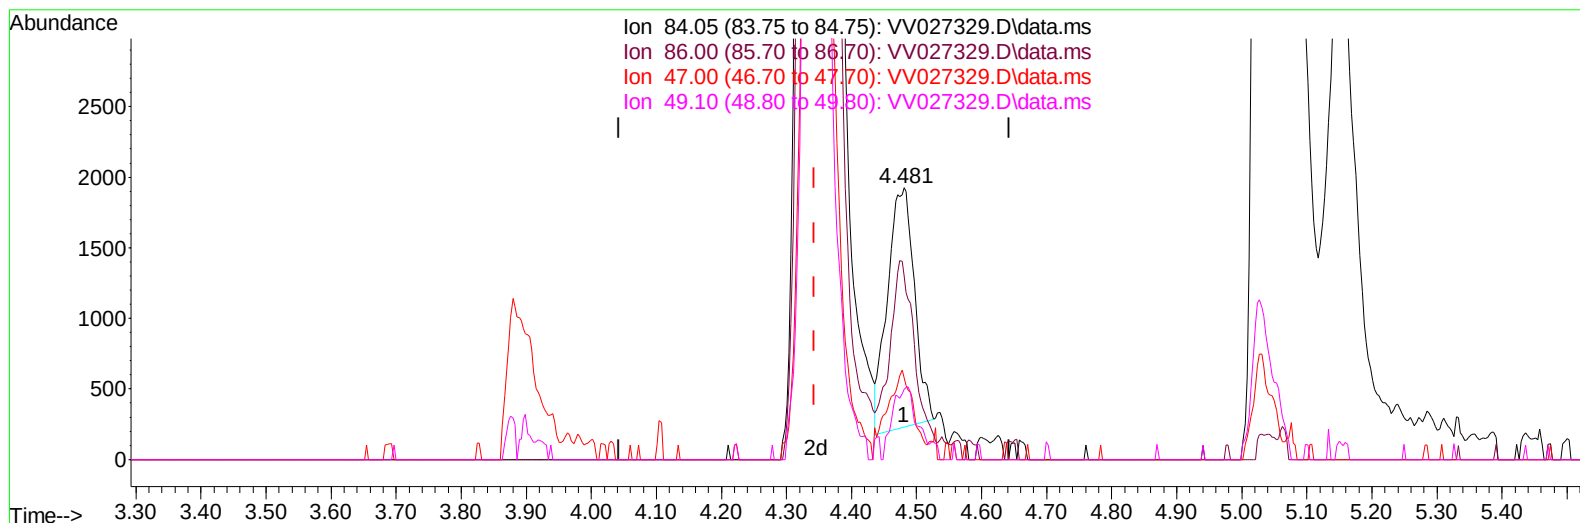

TIC: VV027329.D\data.ms

(24) Chloroform-d (S)

4.481min (+ 0.138) 0.19 ug/L

response 4921

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	62.80	70.47
47.00	45.70	36.27
49.10	27.40	27.27




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027329.D
 Acq On : 12 Aug 2022 13:54
 Operator : SY/MD
 Sample : N4145-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY148

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:37:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

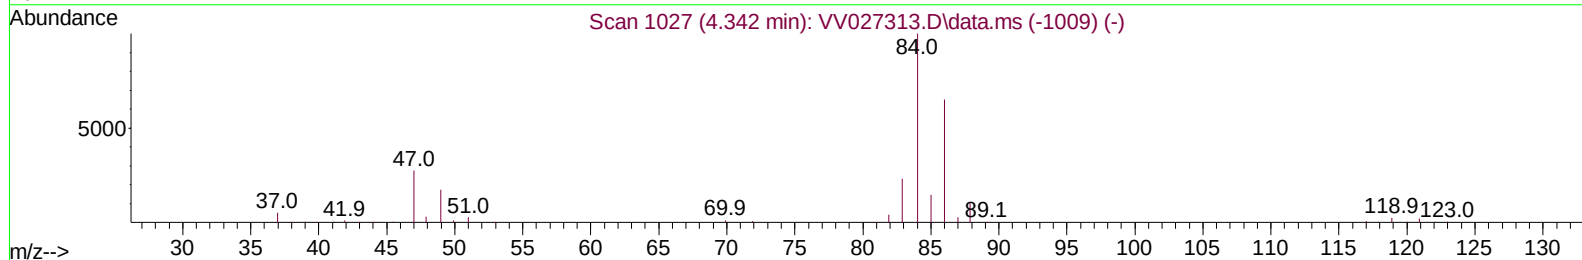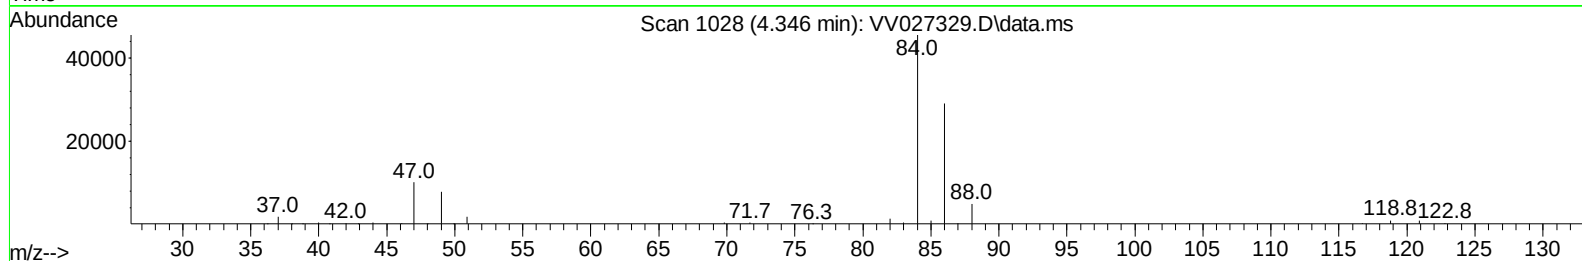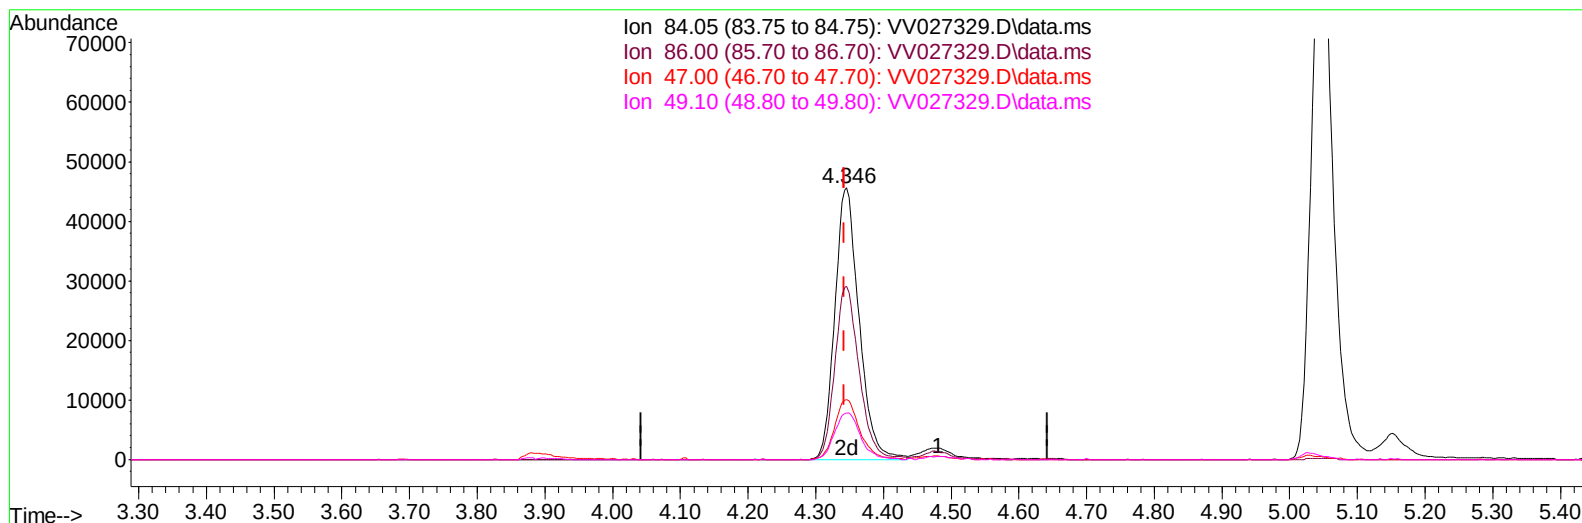

TIC: VV027329.D\data.ms

(24) Chloroform-d (S)

4.346min (+ 0.003) 4.30 ug/L m

response 113025

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	62.80	3.07#
47.00	45.70	1.58#
49.10	27.40	1.19#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027329.D
 Acq On : 12 Aug 2022 13:54
 Operator : SY/MD
 Sample : N4145-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY148

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:37:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	164988	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	178179	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71632	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	58349	4.071	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	81.400%	
7) Chloroethane-d5	1.561	69	40485	3.889	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	77.800%	
11) 1,1-Dichloroethene-d2	2.101	63	77569	2.984	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	59.600%#	
20) 2-Butanone-d5	3.883	46	119906	49.393	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	98.780%	
24) Chloroform-d	4.346	84	113025m	4.299	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	86.000%	
26) 1,2-Dichloroethane-d4	5.031	65	55910	4.464	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	89.200%	
32) Benzene-d6	5.047	84	200947	3.823	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	76.400%	
36) 1,2-Dichloropropane-d6	6.069	67	67009	4.123	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	82.400%	
41) Toluene-d8	7.313	98	164319	3.415	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	68.200%#	
43) trans-1,3-Dichloroprop...	7.625	79	21456	3.812	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	76.200%	
46) 2-Hexanone-d5	8.088	63	79306	36.403	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	72.800%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44655	3.798	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	76.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	57275	4.633	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	92.600%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027329.D
Acq On : 12 Aug 2022 13:54
Operator : SY/MD
Sample : N4145-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY148

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:37:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 08:00:46 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

