




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027330.D
 Acq On : 12 Aug 2022 14:19
 Operator : SY/MD
 Sample : N4145-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7G6

Manual IntegrationsAPPROVED

Quant Time: Aug 13 01:37:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

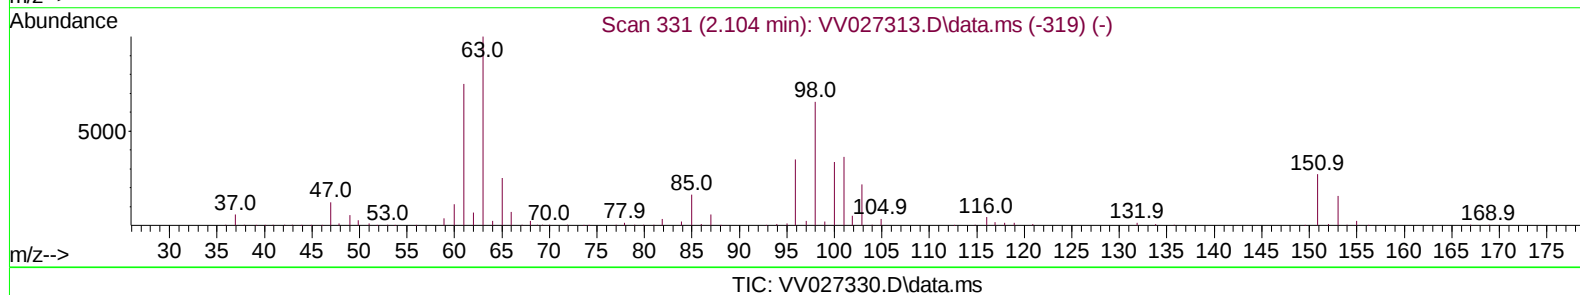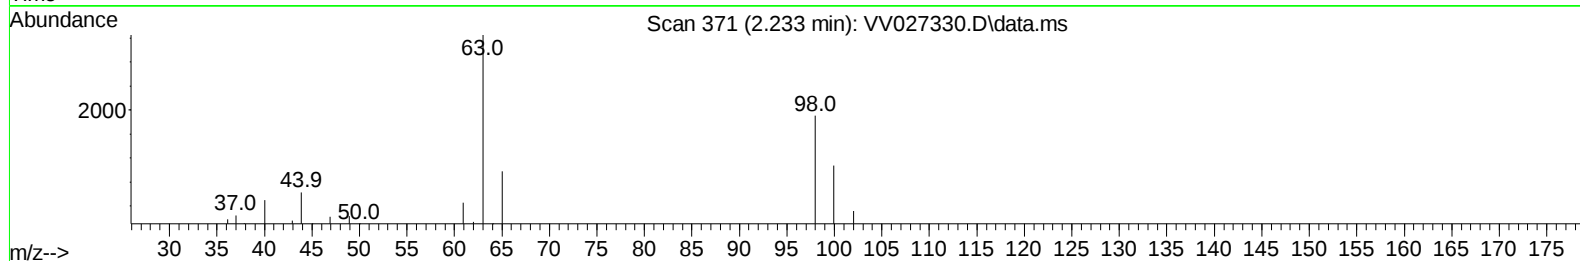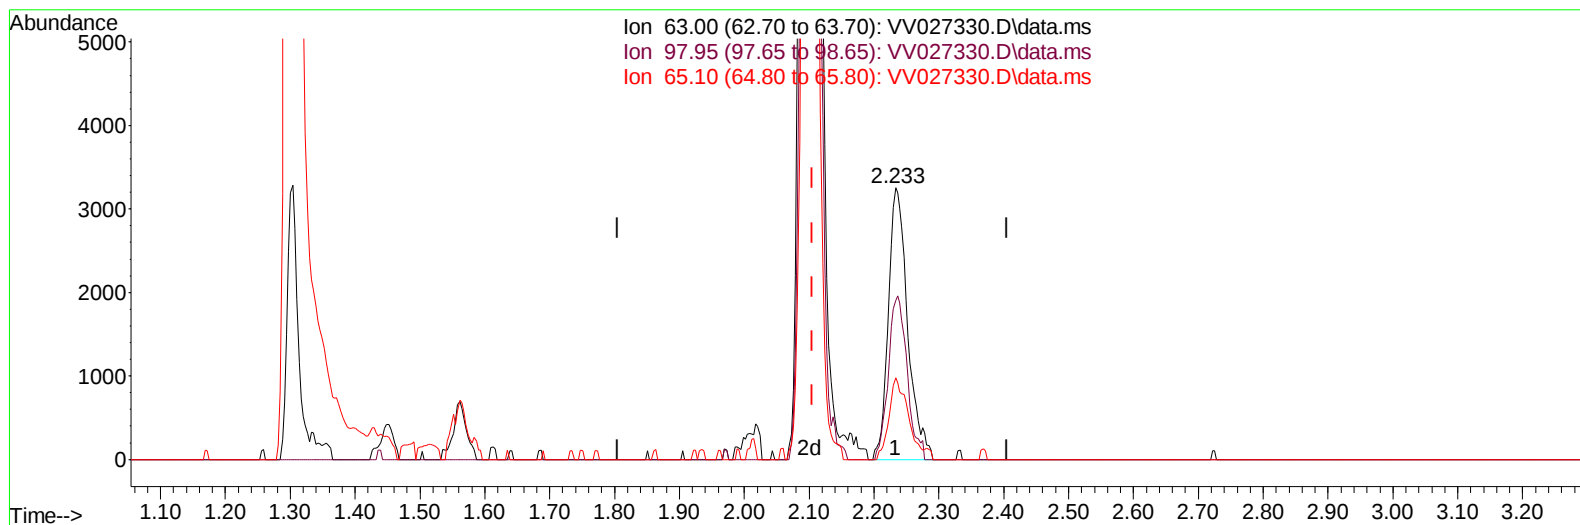

(11) 1,1-Dichloroethene-d2 (S)

2.233min (+ 0.129) 0.27 ug/L

response 6741

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	58.73
65.10	23.50	29.49
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027330.D
Acq On : 12 Aug 2022 14:19
Operator : SY/MD
Sample : N4145-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7G6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:37:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 08:00:46 2022
Response via : Initial Calibration

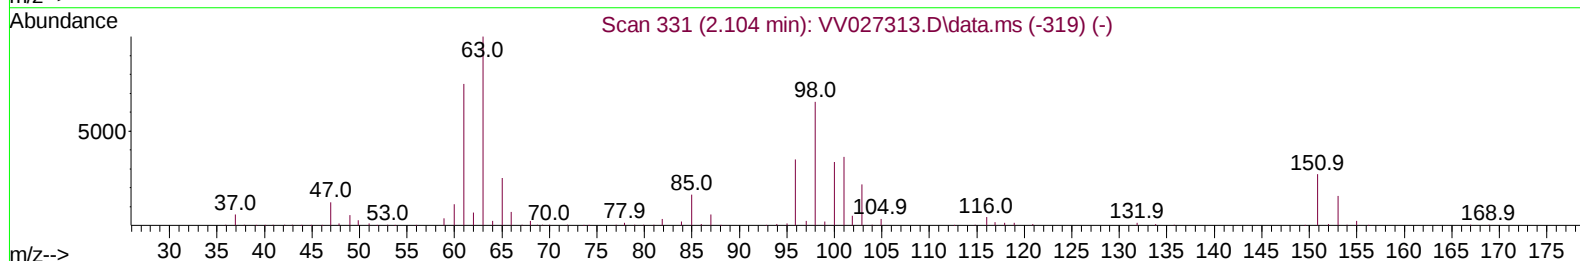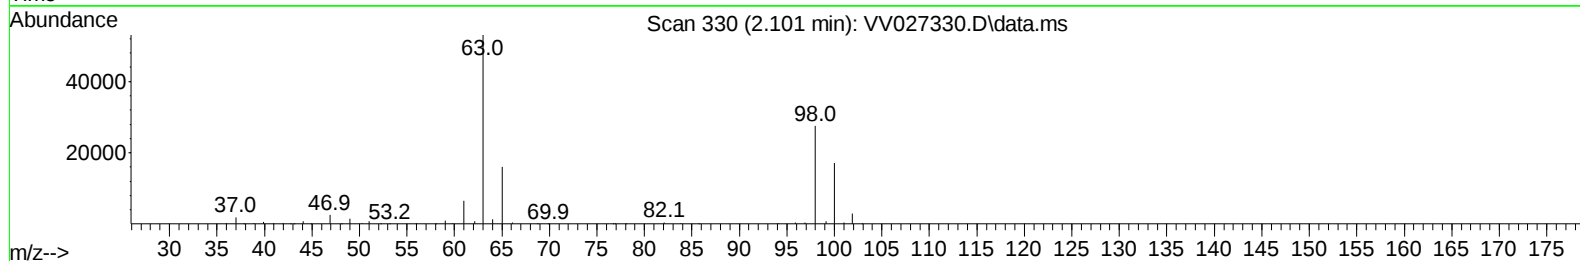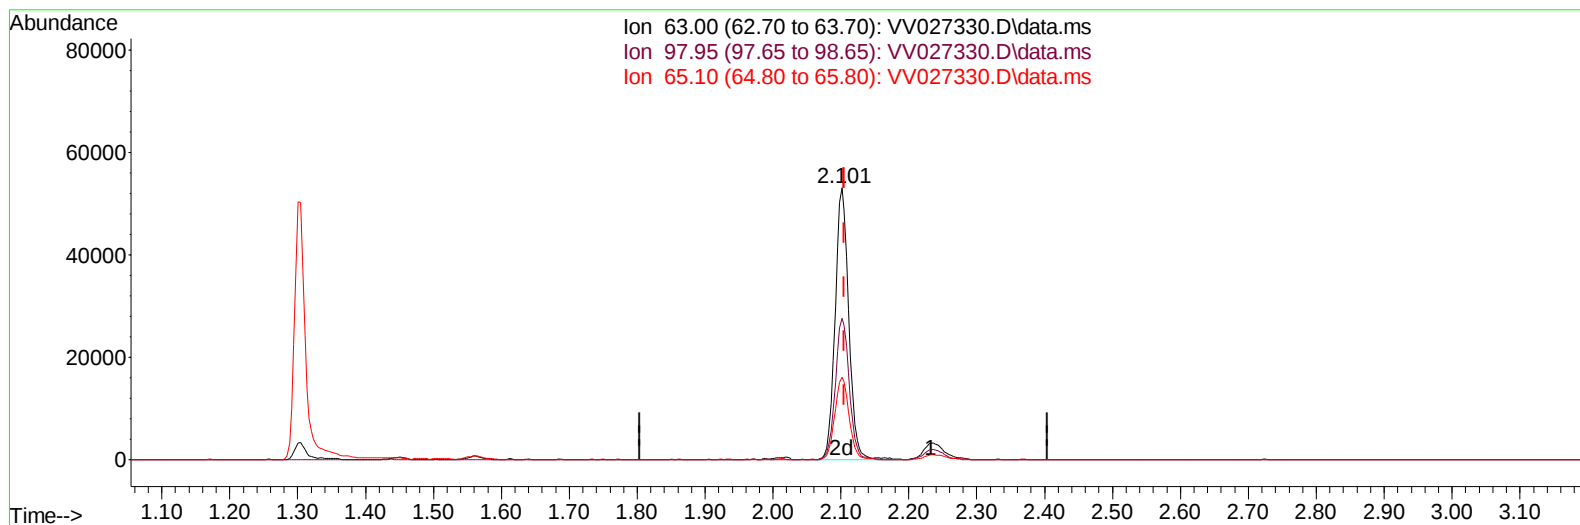

TIC: VV027330.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.003) 2.97 ug/L m

response 73881

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	5.36#
65.10	23.50	2.69#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027330.D
 Acq On : 12 Aug 2022 14:19
 Operator : SY/MD
 Sample : N4145-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7G6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
 Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:37:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	157786	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	171491	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70565	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	57521	4.196	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	84.000%		
7) Chloroethane-d5	1.561	69	42066	4.225	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	84.600%		
11) 1,1-Dichloroethene-d2	2.101	63	73881m	2.972	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	59.400%#		
20) 2-Butanone-d5	3.873	46	115608	49.796	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	99.600%		
24) Chloroform-d	4.346	84	108869	4.330	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	86.600%		
26) 1,2-Dichloroethane-d4	5.027	65	53457	4.463	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	89.200%		
32) Benzene-d6	5.047	84	191372	3.783	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	75.600%		
36) 1,2-Dichloropropane-d6	6.066	67	64812	4.144	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	82.800%		
41) Toluene-d8	7.313	98	157223	3.395	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	67.800%#		
43) trans-1,3-Dichloroprop...	7.625	79	20489	3.782	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	75.600%		
46) 2-Hexanone-d5	8.088	63	78067	37.232	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	74.460%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46185	4.081	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	81.600%		
66) 1,2-Dichlorobenzene-d4	11.625	152	56021	4.600	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	92.000%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027330.D
Acq On : 12 Aug 2022 14:19
Operator : SY/MD
Sample : N4145-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7G6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2022
Supervised By :Mahesh Dadoda 08/14/2022

Quant Time: Aug 13 01:37:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 08:00:46 2022
Response via : Initial Calibration

