

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027305.D
 Acq On : 12 Aug 2022 03:07
 Operator : SY/MD
 Sample : N4162-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBY1

Quant Time: Aug 12 05:48:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 02:11:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	160185	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	173182	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70751	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	72805	5.231	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	104.600%	
7) Chloroethane-d5	1.565	69	53775	5.320	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	106.400%	
11) 1,1-Dichloroethene-d2	2.101	63	97521	3.864	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	77.200%	
20) 2-Butanone-d5	3.886	46	85761	36.387	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	72.780%	
24) Chloroform-d	4.343	84	126138	4.942	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.800%	
26) 1,2-Dichloroethane-d4	5.031	65	60647	4.988	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.800%	
32) Benzene-d6	5.047	84	238189	4.662	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.200%	
36) 1,2-Dichloropropane-d6	6.066	67	80839	5.118	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.400%	
41) Toluene-d8	7.313	98	200485	4.287	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.800%	
43) trans-1,3-Dichloroprop...	7.625	79	23494	4.294	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.800%	
46) 2-Hexanone-d5	8.088	63	86317	40.765	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	81.520%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	50144	4.388	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	64843	5.310	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.200%	
Target Compounds						
					Qvalue	
22) cis-1,2-Dichloroethene	3.912	96	6145	0.440	ug/L	99
29) 1,1,1-Trichloroethane	4.600	97	1774	0.073	ug/L #	84
34) Trichloroethene	5.915	95	32055	2.176	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027305.D
Acq On : 12 Aug 2022 03:07
Operator : SY/MD
Sample : N4162-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY1

Quant Time: Aug 12 05:48:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 02:11:44 2022
Response via : Initial Calibration




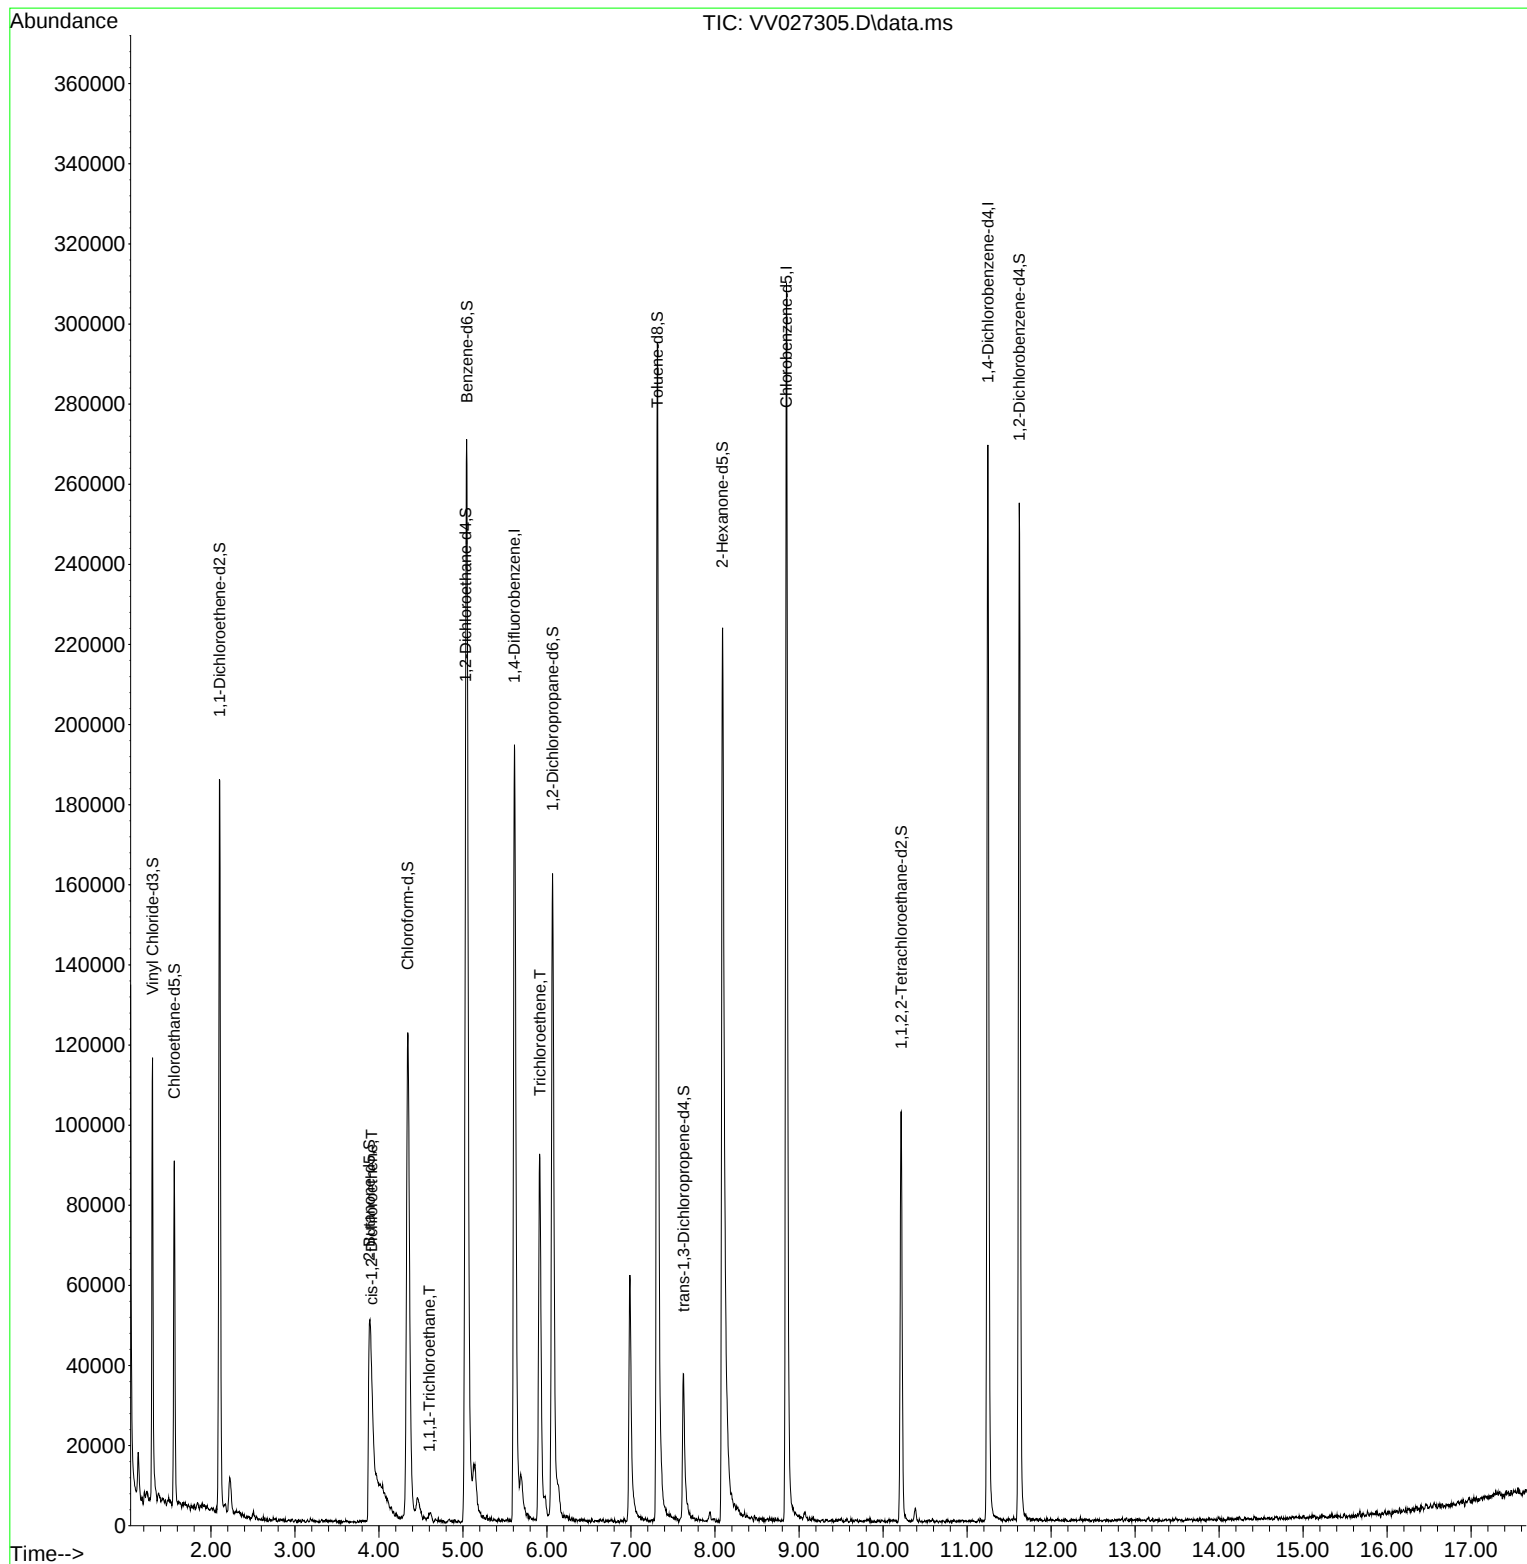


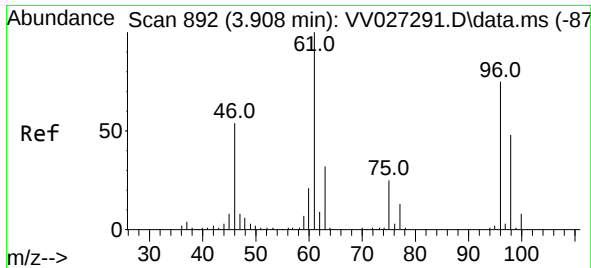

#22
 cis-1,2-Dichloroethene
 Concen: 0.440 ug/L
 RT: 3.912 min Scan# 892
 Delta R.T. 0.003 min
 Lab File: VV027305.D
 Acq: 12 Aug 2022 03:07




Instrument :
 MSVOA_V
 ClientSampleId :
 BGBY1


Tgt Ion: 96 Resp: 6145
 Ion Ratio Lower Upper
 96 100
 61 129.7 91.3 169.5
 68 0.0 0.0 0.0

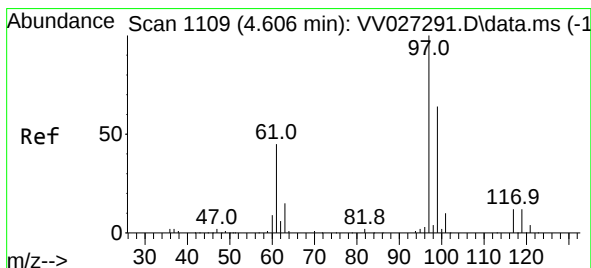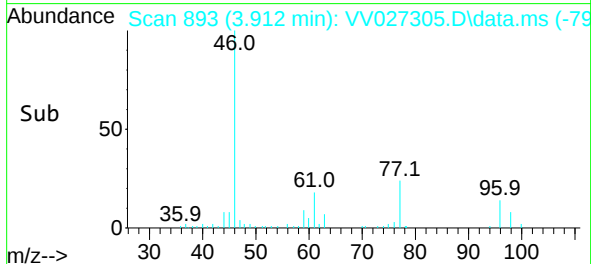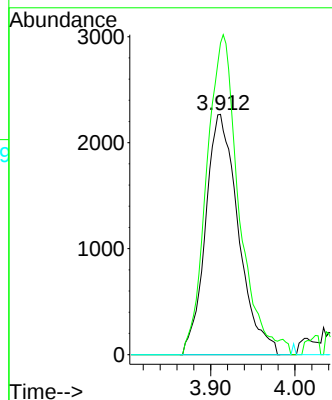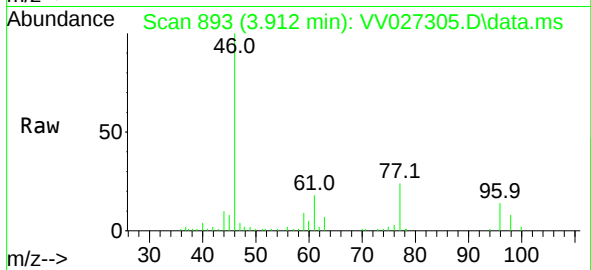

#29
 1,1,1-Trichloroethane
 Concen: 0.073 ug/L
 RT: 4.600 min Scan# 1107
 Delta R.T. -0.006 min
 Lab File: VV027305.D
 Acq: 12 Aug 2022 03:07


Tgt Ion: 97 Resp: 1774
 Ion Ratio Lower Upper
 97 100
 99 64.4 50.8 76.2
 61 21.1 36.5 54.7#

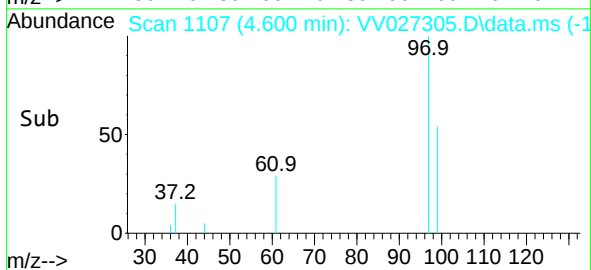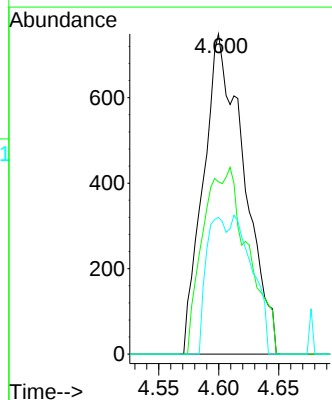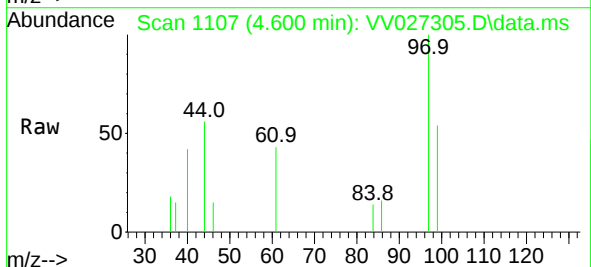

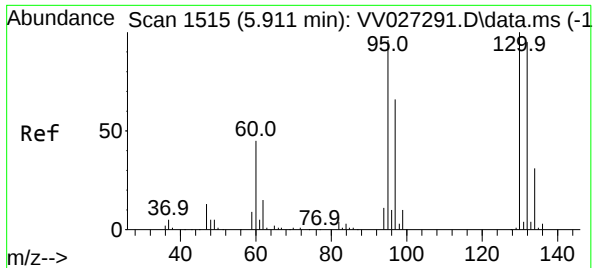

#34
 Trichloroethene
 Concen: 2.176 ug/L
 RT: 5.915 min Scan# 11
 Delta R.T. 0.003 min
 Lab File: VV027305.D
 Acq: 12 Aug 2022 03:07

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBY1

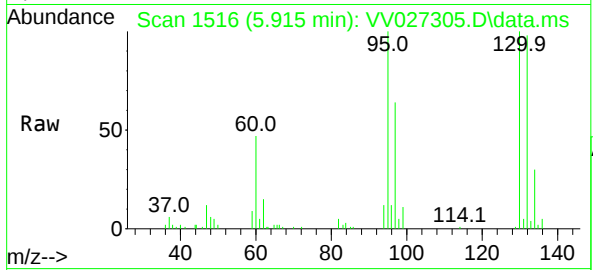

Tgt Ion: 95	Resp: 32055
Ion Ratio	Lower Upper
95 100	
97 64.0	45.5 84.5
132 98.1	68.2 126.6
130 99.9	70.3 130.7

