

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027309.D
 Acq On : 12 Aug 2022 04:46
 Operator : SY/MD
 Sample : N4162-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX0

Quant Time: Aug 12 05:49:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 02:11:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	150420	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	164730	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67166	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	74666	5.713	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	114.200%
7) Chloroethane-d5	1.564	69	53545	5.642	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.800%
11) 1,1-Dichloroethene-d2	2.105	63	96250	4.061	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.200%
20) 2-Butanone-d5	3.880	46	116643	52.703	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.400%
24) Chloroform-d	4.346	84	127167	5.306	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.200%
26) 1,2-Dichloroethane-d4	5.031	65	63042	5.521	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	5.047	84	236123	4.859	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
36) 1,2-Dichloropropane-d6	6.066	67	80480	5.356	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.200%
41) Toluene-d8	7.313	98	195095	4.385	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
43) trans-1,3-Dichloroprop...	7.622	79	22523	4.328	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.600%
46) 2-Hexanone-d5	8.088	63	83397	41.407	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.820%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	49865	4.587	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	63252	5.456	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.200%
Target Compounds						Qvalue
34) Trichloroethene	5.918	95	7029	0.502	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027309.D
Acq On : 12 Aug 2022 04:46
Operator : SY/MD
Sample : N4162-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX0


Quant Time: Aug 12 05:49:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 02:11:44 2022
Response via : Initial Calibration

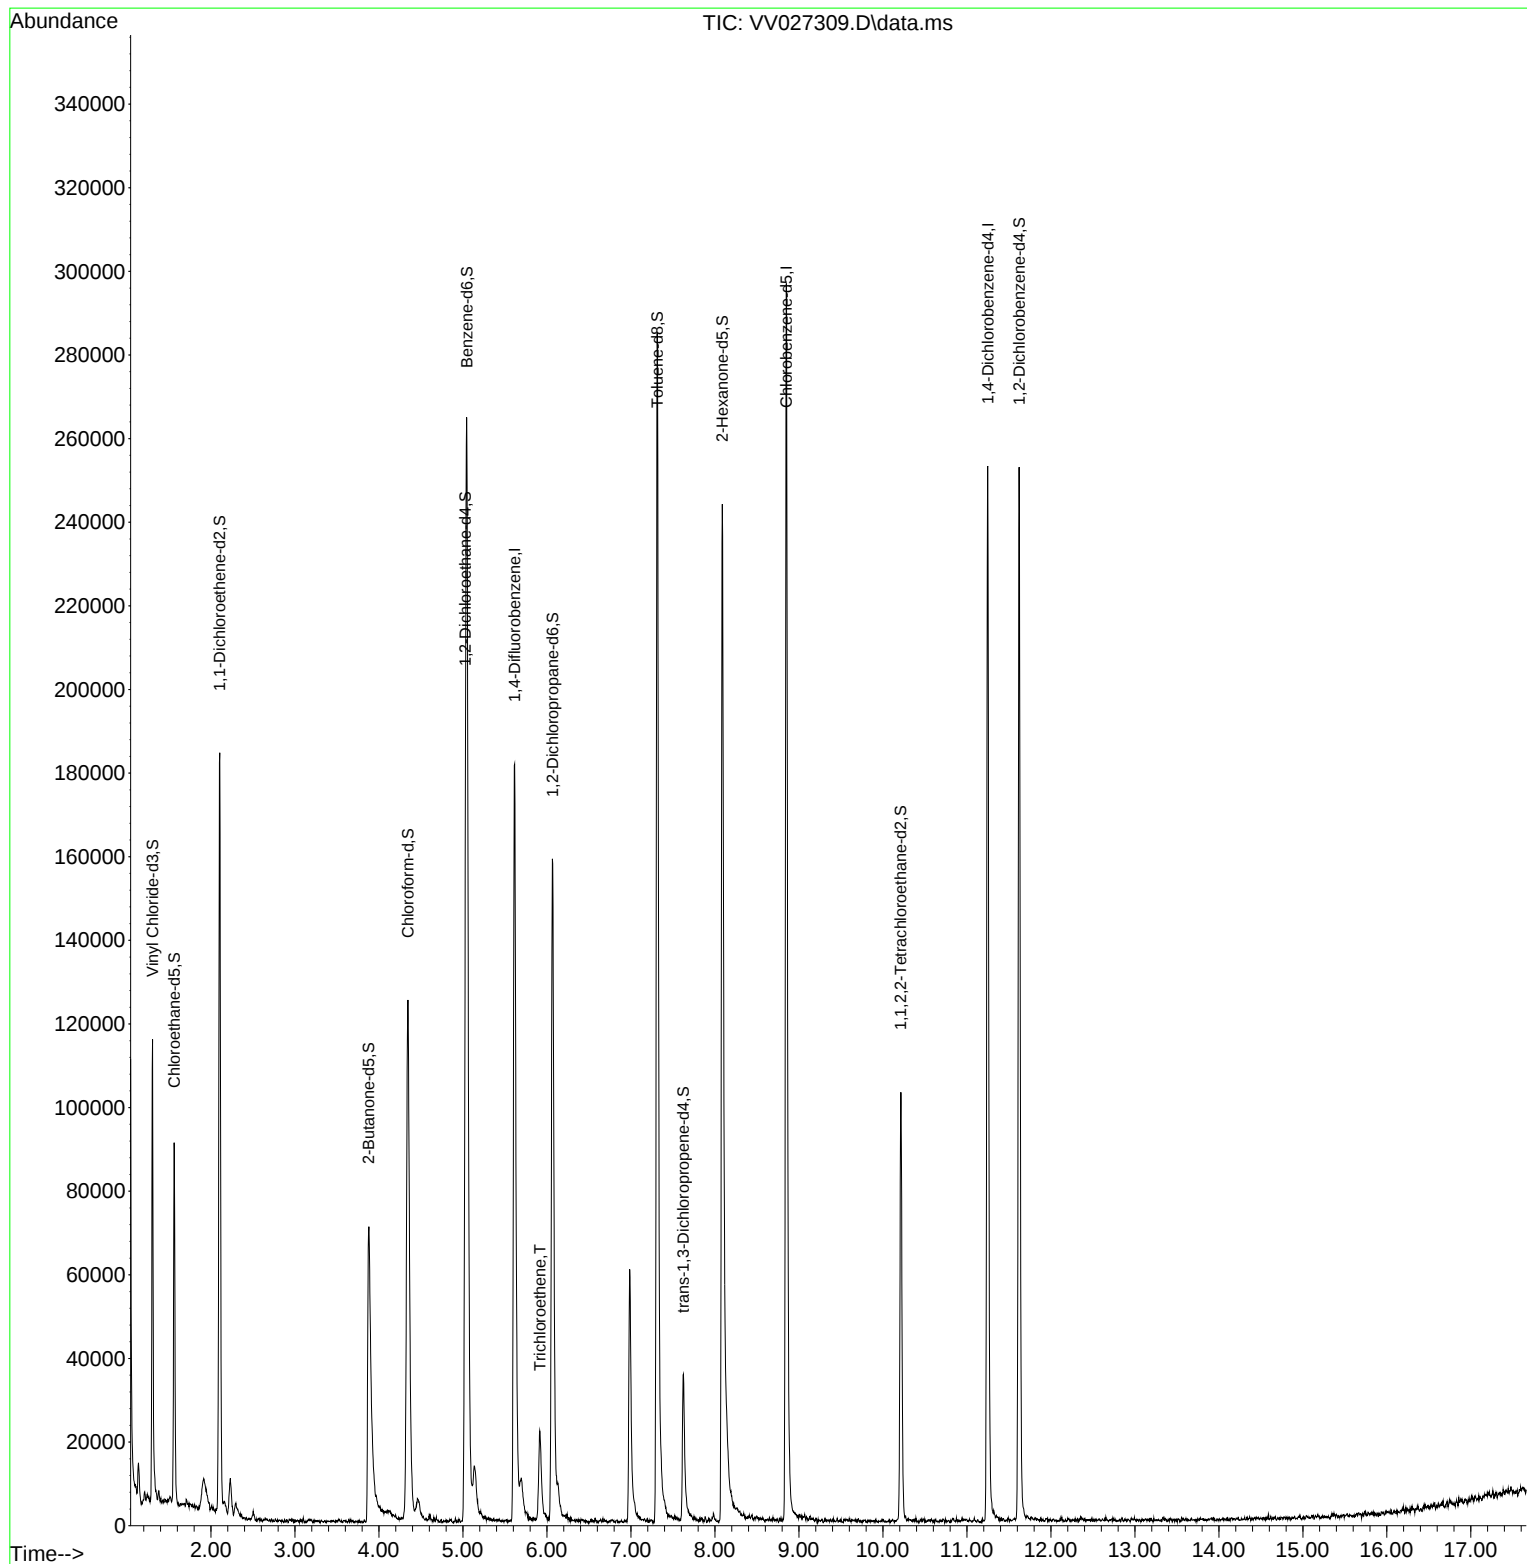

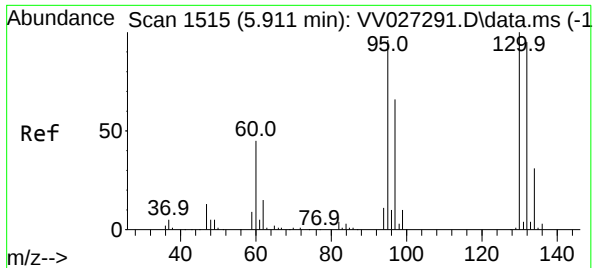

#34
 Trichloroethene
 Concen: 0.502 ug/L
 RT: 5.918 min Scan# 11
 Delta R.T. 0.007 min
 Lab File: VV027309.D
 Acq: 12 Aug 2022 04:46

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX0

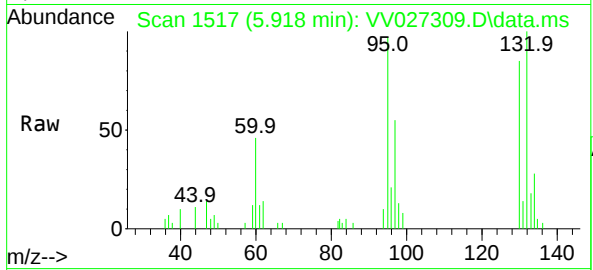

Tgt Ion: 95 Resp: 7029

Ion	Ratio	Lower	Upper
95	100		
97	56.7	45.5	84.5
132	103.1	68.2	126.6
130	88.0	70.3	130.7

