

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027325.D
 Acq On : 12 Aug 2022 12:14
 Operator : SY/MD
 Sample : N4164-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC12

Quant Time: Aug 13 01:36:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 08:00:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	147459	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	162766	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63835	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	68713	5.363	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.200%
7) Chloroethane-d5	1.564	69	49386	5.308	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.200%
11) 1,1-Dichloroethene-d2	2.101	63	87591	3.770	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.400%
20) 2-Butanone-d5	3.889	46	95653	44.086	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.180%
24) Chloroform-d	4.346	84	123225	5.245	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%
26) 1,2-Dichloroethane-d4	5.030	65	59688	5.332	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	5.047	84	226484	4.717	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%
36) 1,2-Dichloropropane-d6	6.066	67	72513	4.884	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.313	98	186359	4.240	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.800%
43) trans-1,3-Dichloroprop...	7.625	79	20377	3.963	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.088	63	80754	40.578	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.160%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47993	4.469	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	61015	5.538	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.800%
Target Compounds					Qvalue	
13) Acetone	2.172	43	16128	10.059	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027325.D
Acq On : 12 Aug 2022 12:14
Operator : SY/MD
Sample : N4164-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC12

Quant Time: Aug 13 01:36:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 08:00:46 2022
Response via : Initial Calibration

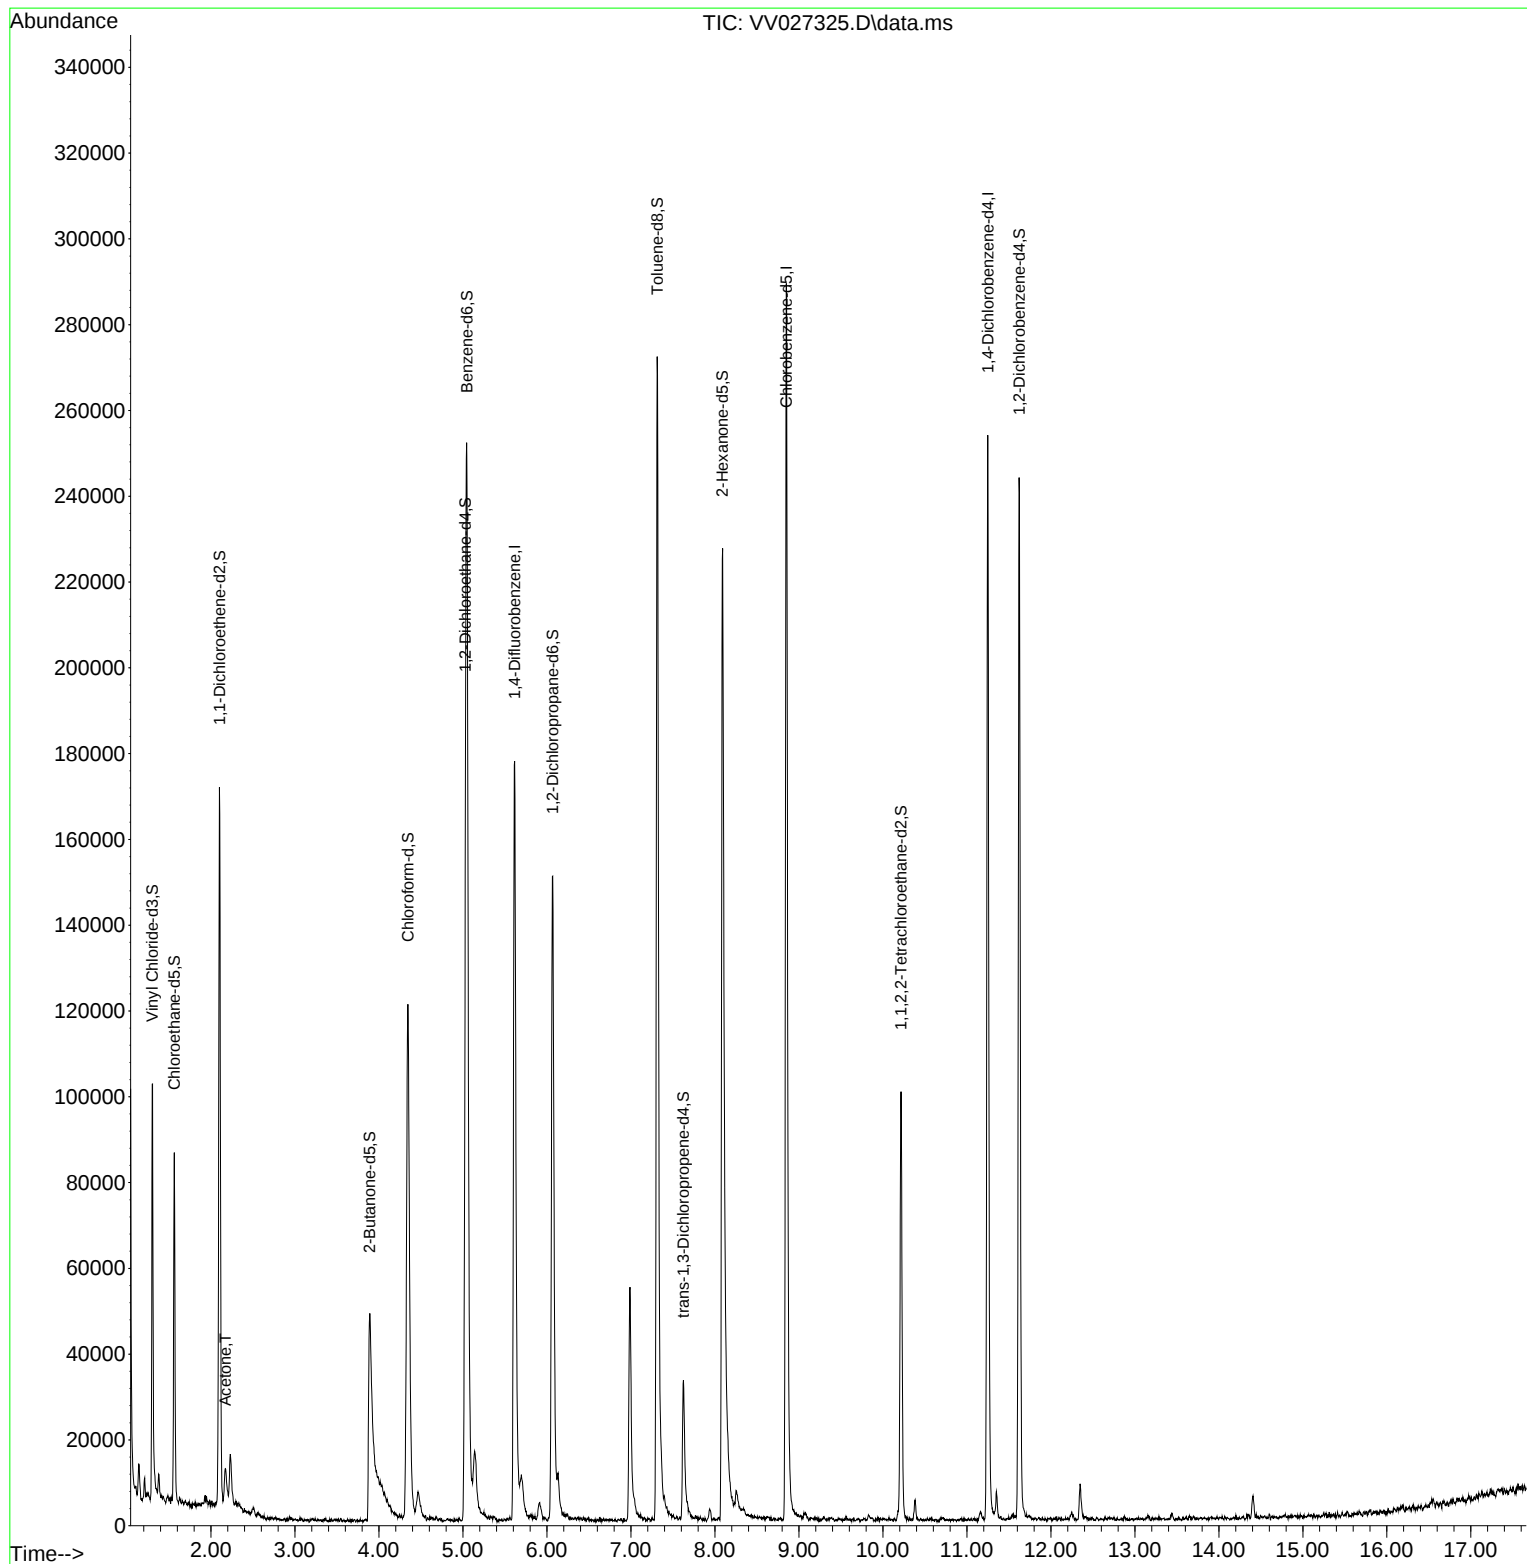

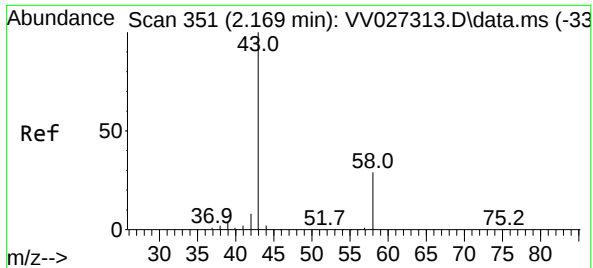

#13
 Acetone
 Concen: 10.059 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV027325.D
 Acq: 12 Aug 2022 12:14

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC12

Tgt Ion: 43 Resp: 16128
 Ion Ratio Lower Upper
 43 100
 58 28.6 0.0 63.2

