

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027336.D
 Acq On : 12 Aug 2022 18:45
 Operator : SY/MD
 Sample : VV0812WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Quant Time: Aug 13 02:48:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 13 02:46:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	171674	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	176468	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	74996	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	62839	4.213	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.200%
7) Chloroethane-d5	1.561	69	46637	4.305	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.200%
11) 1,1-Dichloroethene-d2	2.101	63	85216	3.150	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.000%
20) 2-Butanone-d5	3.883	46	93683	37.088	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	74.180%
24) Chloroform-d	4.343	84	119399	4.365	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
26) 1,2-Dichloroethane-d4	5.027	65	60637	4.653	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.000%
32) Benzene-d6	5.043	84	236917	4.551	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
36) 1,2-Dichloropropane-d6	6.063	67	73480	4.565	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.400%
41) Toluene-d8	7.314	98	203981	4.280	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%
43) trans-1,3-Dichloroprop...	7.622	79	25565	4.585	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.800%
46) 2-Hexanone-d5	8.088	63	86924	40.287	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.580%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48310	4.149	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	65433	5.055	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.000%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	7377	0.372	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027336.D
Acq On : 12 Aug 2022 18:45
Operator : SY/MD
Sample : VV0812WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Quant Time: Aug 13 02:48:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 02:46:03 2022
Response via : Initial Calibration

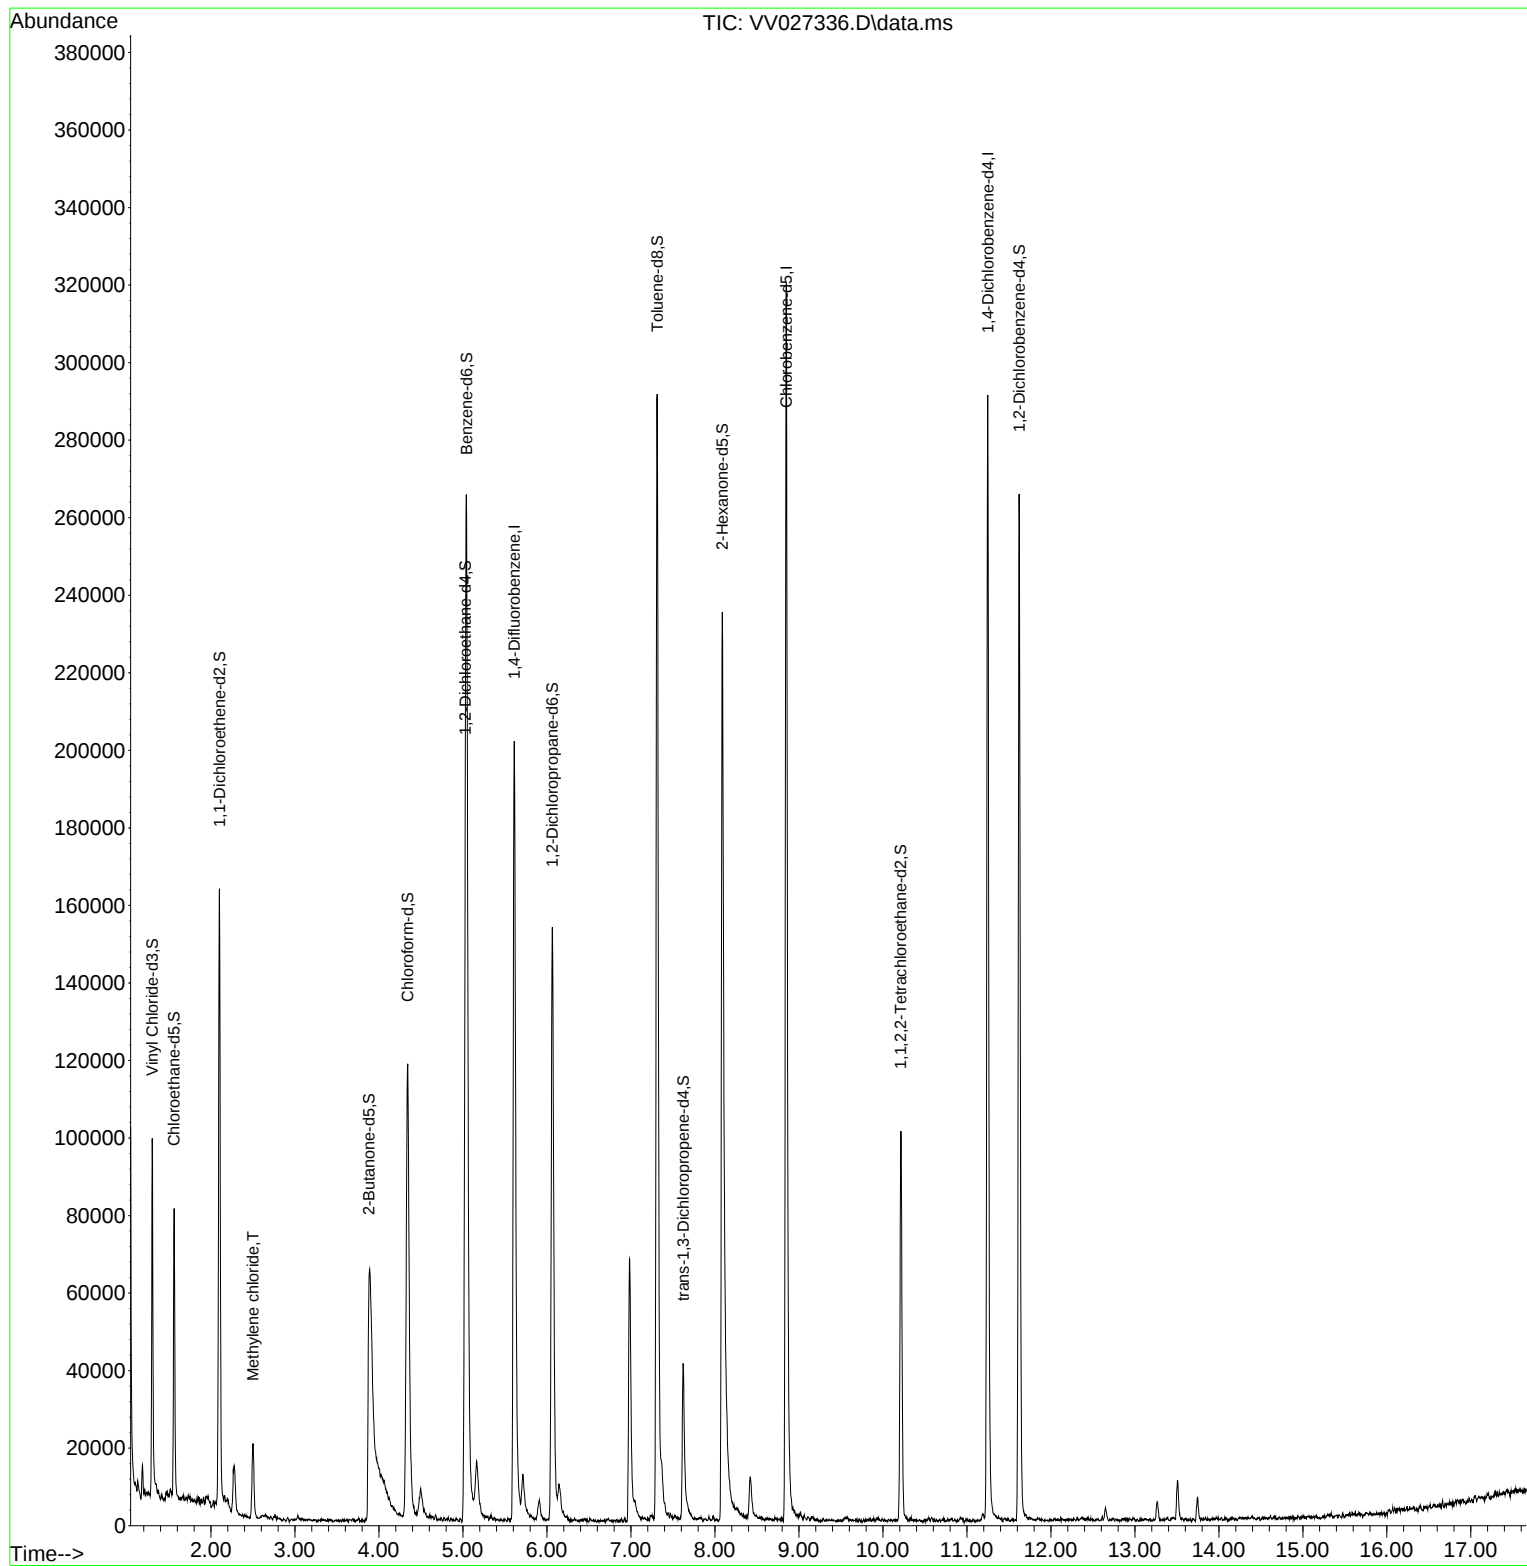

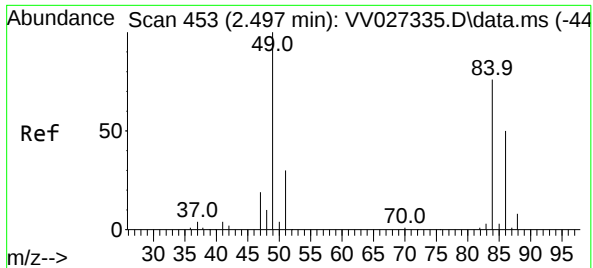

#16
Methylene chloride
Concen: 0.372 ug/L
RT: 2.500 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV027336.D
Acq: 12 Aug 2022 18:45

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Tgt Ion:	84	Resp:	7377
Ion	Ratio	Lower	Upper
84	100		
86	68.3	45.1	83.9
49	125.6	91.2	169.4

