

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027338.D
 Acq On : 12 Aug 2022 20:00
 Operator : SY/MD
 Sample : N4133-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E62

Quant Time: Aug 13 04:16:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 13 02:46:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	157220	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	164491	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75378	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	49765	3.643	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.800%
7) Chloroethane-d5	1.561	69	38434	3.874	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.400%
11) 1,1-Dichloroethene-d2	2.102	63	65304	2.636	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	52.800%#
20) 2-Butanone-d5	3.876	46	128902	55.722	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.440%
24) Chloroform-d	4.346	84	102829	4.105	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.000%
26) 1,2-Dichloroethane-d4	5.031	65	50851	4.261	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.047	84	181096	3.732	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.600%
36) 1,2-Dichloropropane-d6	6.066	67	61165	4.077	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.600%
41) Toluene-d8	7.314	98	145976	3.286	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	65.800%#
43) trans-1,3-Dichloroprop...	7.625	79	20051	3.858	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.200%
46) 2-Hexanone-d5	8.088	63	82050	40.797	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.600%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46073	4.245	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	60910	4.682	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.600%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.500	84	18506	1.018	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027338.D
Acq On : 12 Aug 2022 20:00
Operator : SY/MD
Sample : N4133-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E62

Quant Time: Aug 13 04:16:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 02:46:03 2022
Response via : Initial Calibration

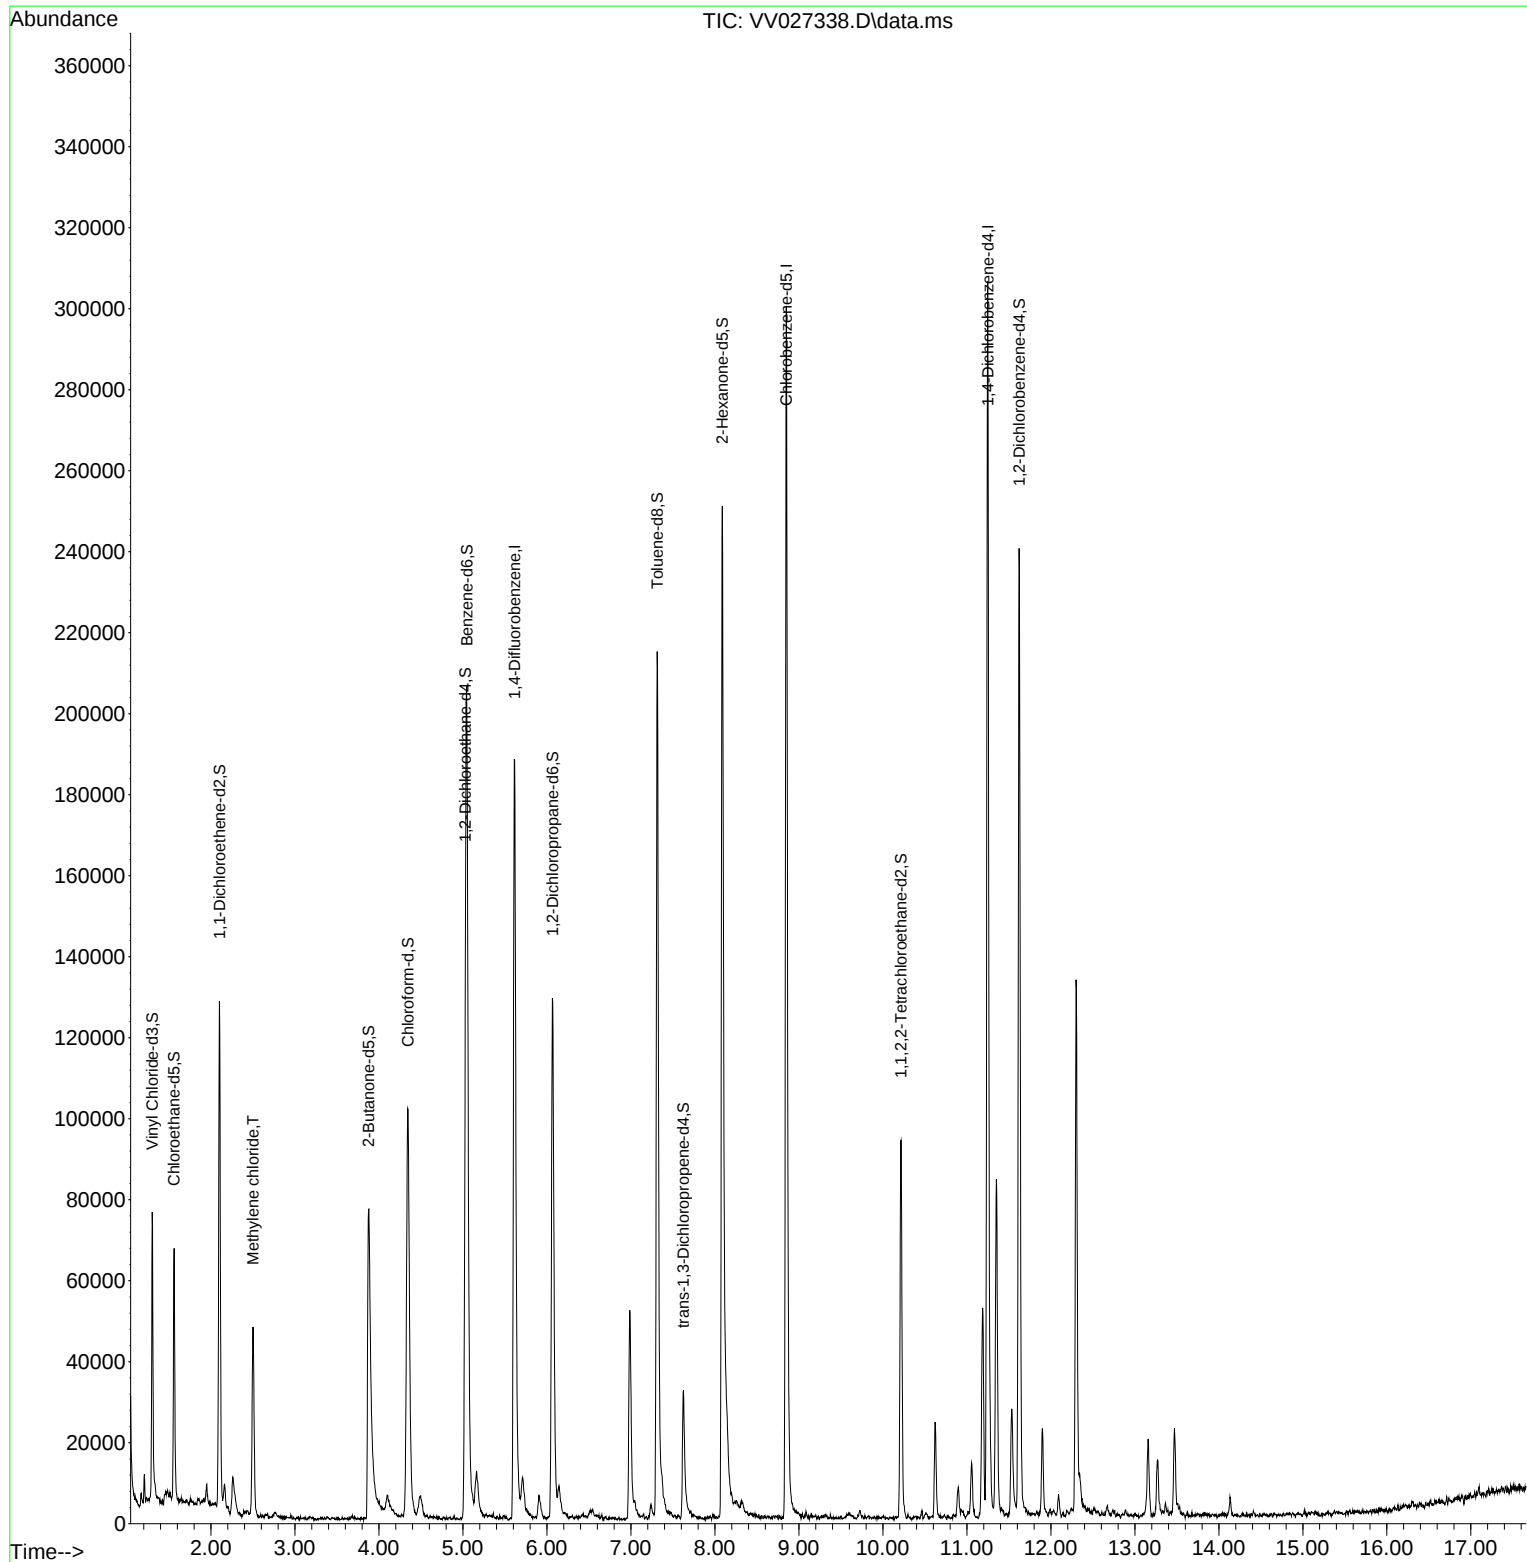

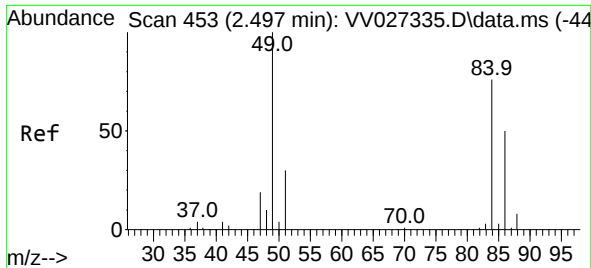

#16
Methylene chloride
Concen: 1.018 ug/L
RT: 2.500 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV027338.D
Acq: 12 Aug 2022 20:00

Instrument :
MSVOA_V
ClientSampleId :
F5E62

Tgt Ion: 84 Resp: 18506
Ion Ratio Lower Upper
84 100
86 59.9 45.1 83.9
49 123.2 91.2 169.4

