

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027352.D
 Acq On : 13 Aug 2022 01:49
 Operator : SY/MD
 Sample : VIBLK277
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK277

Quant Time: Aug 13 04:19:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 13 02:46:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	142175	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	148505	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58780	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	47991	3.885	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%
7) Chloroethane-d5	1.561	69	38931	4.340	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.800%
11) 1,1-Dichloroethene-d2	2.101	63	61726	2.755	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.200%#
20) 2-Butanone-d5	3.873	46	121685	58.169	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.340%
24) Chloroform-d	4.342	84	101834	4.495	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	5.027	65	49970	4.630	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
32) Benzene-d6	5.047	84	172114	3.929	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.600%
36) 1,2-Dichloropropane-d6	6.066	67	59224	4.372	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.400%
41) Toluene-d8	7.313	98	133773	3.336	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.800%#
43) trans-1,3-Dichloroprop...	7.625	79	14838	3.163	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.200%
46) 2-Hexanone-d5	8.085	63	83384	45.923	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.840%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	46714	4.767	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	48922	4.822	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	6545	0.398	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027352.D
Acq On : 13 Aug 2022 01:49
Operator : SY/MD
Sample : VIBLK277
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Quant Time: Aug 13 04:19:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 02:46:03 2022
Response via : Initial Calibration

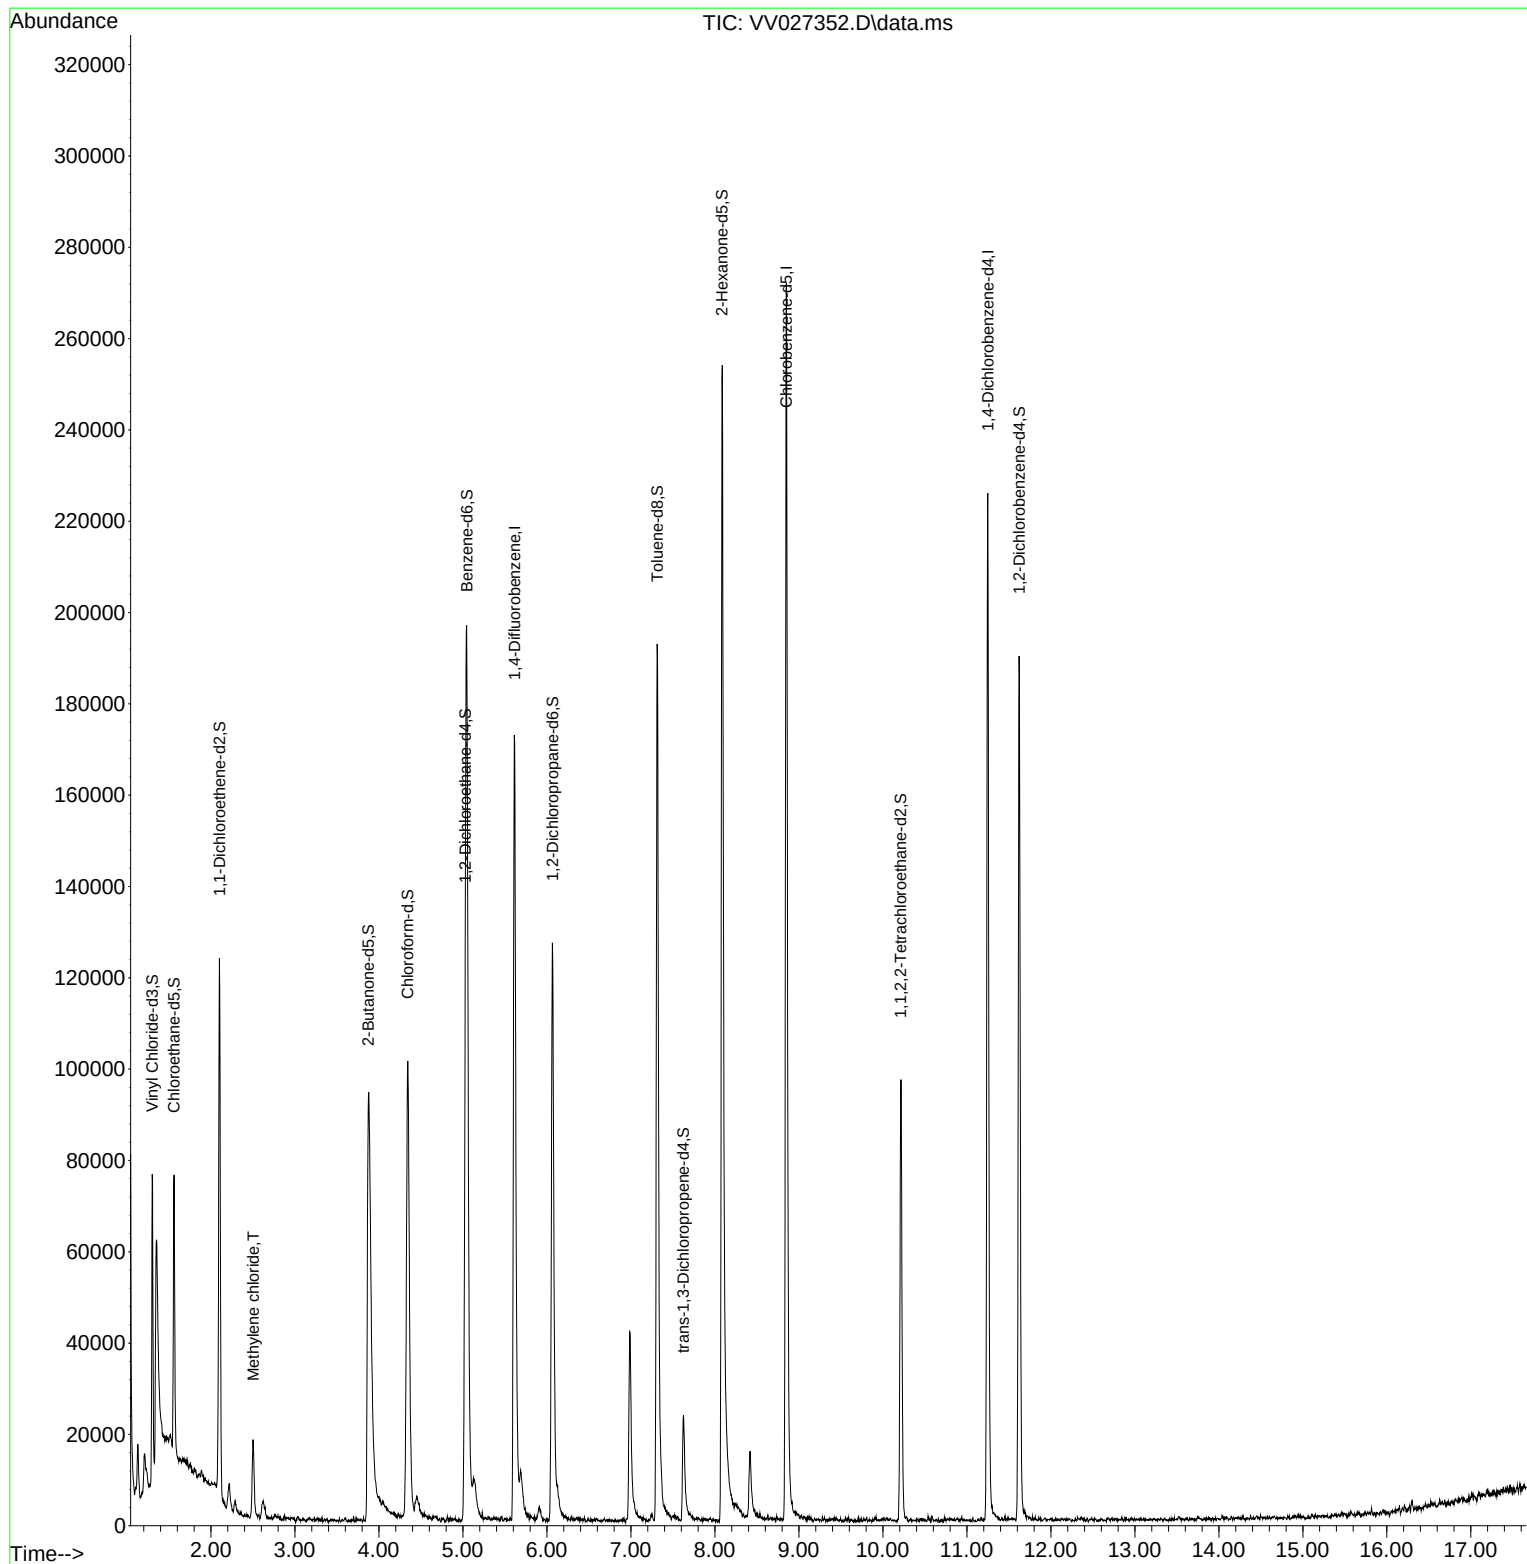

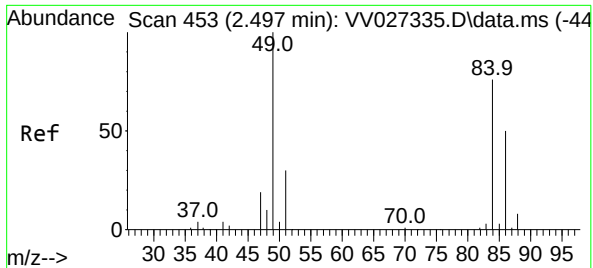

#16
Methylene chloride
Concen: 0.398 ug/L
RT: 2.503 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV027352.D
Acq: 13 Aug 2022 01:49

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Tgt Ion:	84	Resp:	6545
Ion	Ratio	Lower	Upper
84	100		
86	65.2	45.1	83.9
49	121.3	91.2	169.4

