

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027295.D
 Acq On : 11 Aug 2022 22:57
 Operator : SY/MD
 Sample : N4161-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC13

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	35	40	48	rVB	6988	7665	1.11%	0.142%
2	1.301	74	81	101	rVB	110768	121325	17.53%	2.244%
3	1.561	155	162	175	rVB	87565	102055	14.74%	1.887%
4	2.101	321	330	346	rVV	187685	268905	38.85%	4.973%
5	2.259	370	379	395	rVB3	10438	21049	3.04%	0.389%
6	3.889	877	886	911	rBV2	44484	150695	21.77%	2.787%
7	4.342	1010	1027	1054	rBV	124103	317288	45.84%	5.868%
8	4.490	1063	1073	1089	rVB4	4850	12577	1.82%	0.233%
9	5.043	1229	1245	1267	rBV2	278126	692174	100.00%	12.801%
10	5.159	1272	1281	1297	rVB4	11466	30303	4.38%	0.560%
11	5.616	1411	1423	1444	rBV	194952	412512	59.60%	7.629%
12	5.709	1446	1452	1463	rVB4	7642	16632	2.40%	0.308%
13	6.066	1551	1563	1580	rBV	163010	337624	48.78%	6.244%
14	6.985	1835	1849	1865	rBV	66425	130134	18.80%	2.407%
15	7.313	1936	1951	1990	rBV	307033	563964	81.48%	10.430%
16	7.622	2038	2047	2064	rBV	39610	77005	11.13%	1.424%
17	8.092	2181	2193	2238	rBV	229686	578469	83.57%	10.698%
18	8.850	2417	2429	2456	rBV	309666	535943	77.43%	9.912%
19	10.217	2842	2854	2866	rBV	108685	173500	25.07%	3.209%
20	11.249	3162	3175	3200	rBV	264910	432543	62.49%	7.999%
21	11.625	3279	3292	3312	rBV	263597	424795	61.37%	7.856%




Sum of corrected areas: 5407157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027295.D
Acq On : 11 Aug 2022 22:57
Operator : SY/MD
Sample : N4161-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

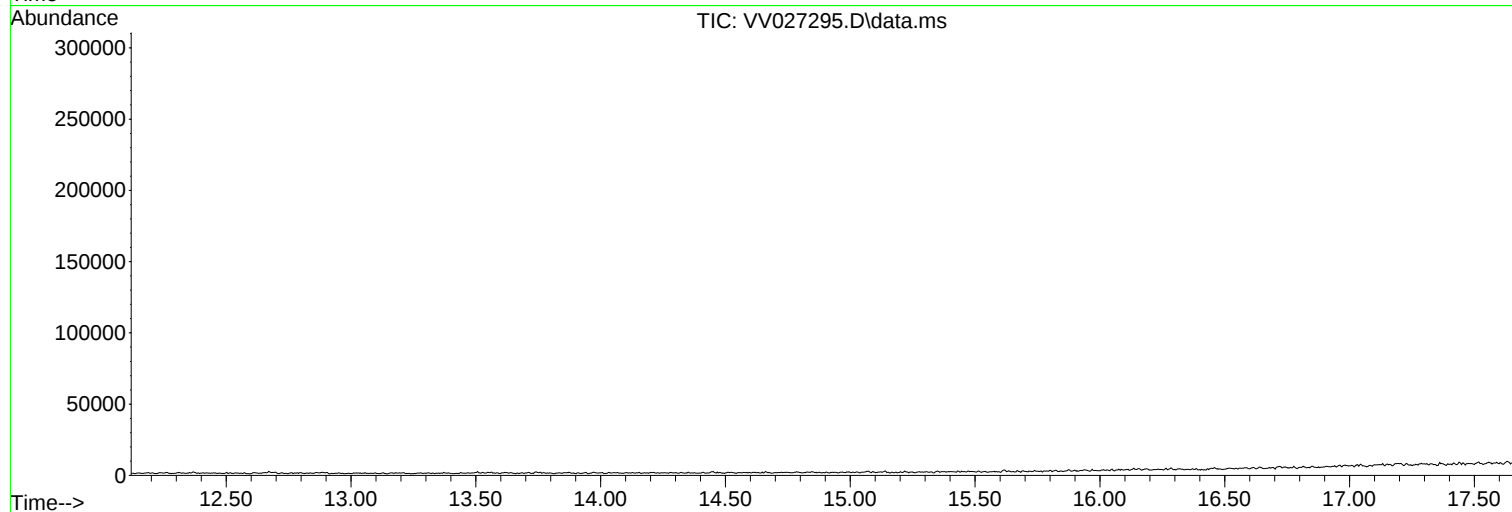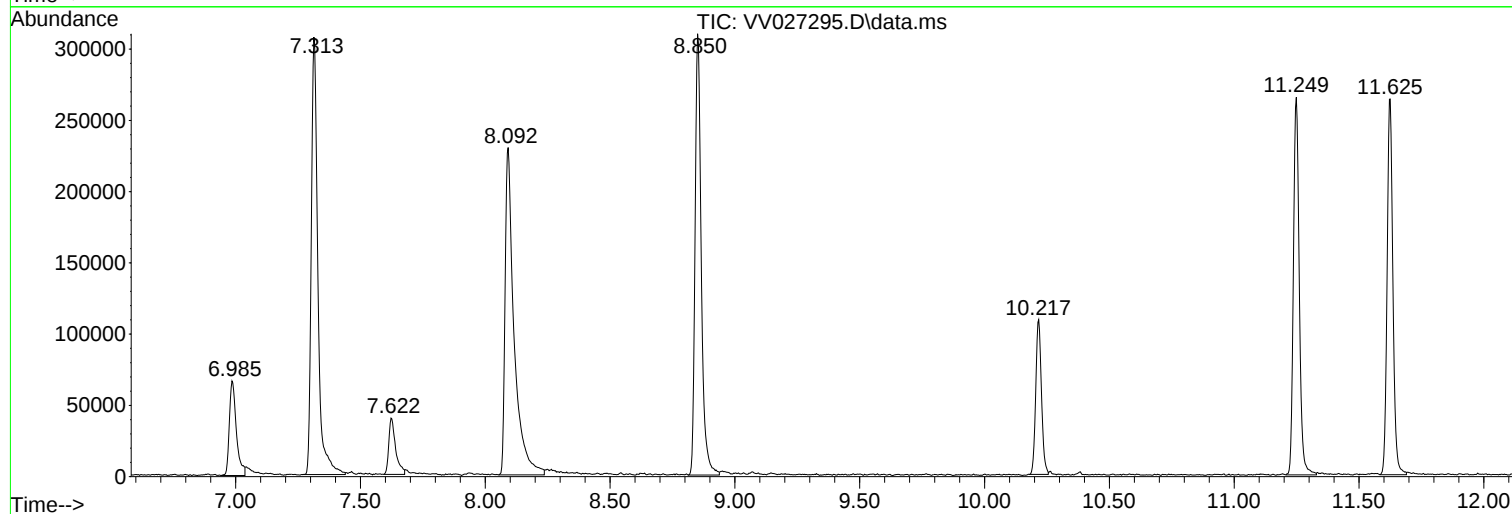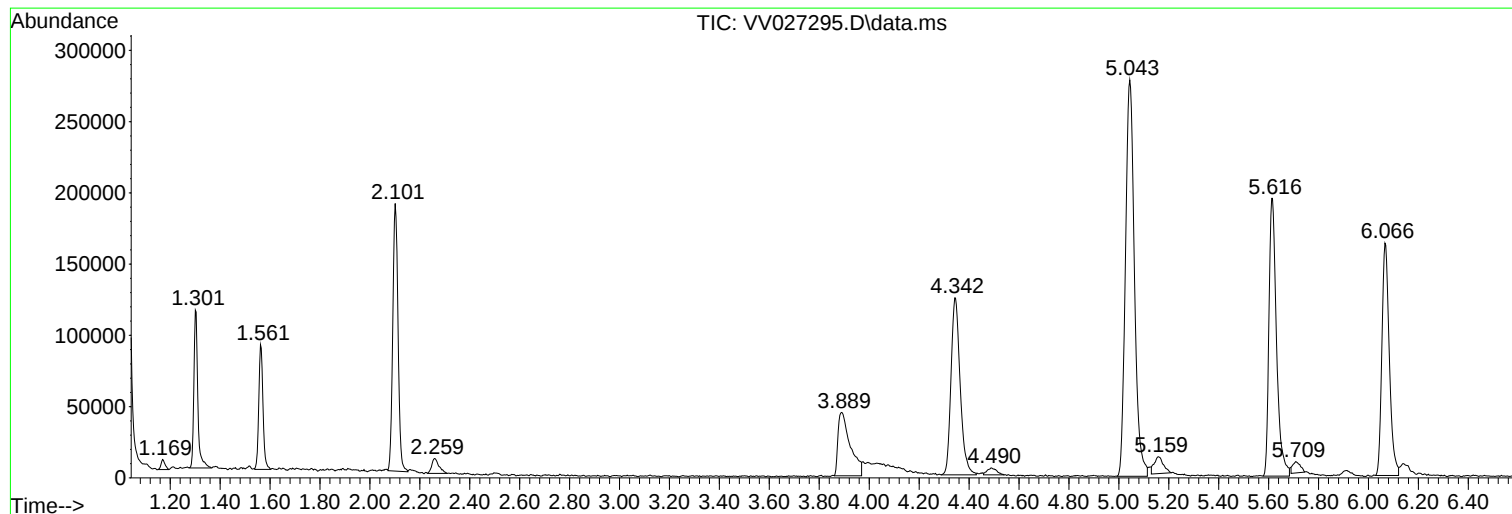

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027295.D
Acq On : 11 Aug 2022 22:57
Operator : SY/MD
Sample : N4161-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027295.D
Acq On : 11 Aug 2022 22:57
Operator : SY/MD
Sample : N4161-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc