

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027298.D
 Acq On : 12 Aug 2022 00:12
 Operator : SY/MD
 Sample : N4162-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC18

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027298.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	73	81	101	rVB	105900	124756	18.66%	2.399%
2	1.564	154	163	179	rVB	83996	99104	14.82%	1.906%
3	2.101	320	330	346	rBV	179022	257594	38.52%	4.954%
4	2.256	369	378	387	rBV2	9744	17417	2.60%	0.335%
5	2.500	442	454	464	rBV6	4610	8824	1.32%	0.170%
6	3.889	876	886	913	rBV	41629	141662	21.19%	2.724%
7	4.346	1011	1028	1051	rBV	121864	320470	47.93%	6.163%
8	4.484	1059	1071	1072	rBV5	5062	6809	1.02%	0.131%
9	5.043	1228	1245	1268	rBV2	266578	668651	100.00%	12.859%
10	5.156	1273	1280	1300	rVB5	13275	32893	4.92%	0.633%
11	5.616	1408	1423	1443	rBV2	188746	395921	59.21%	7.614%
12	5.905	1503	1513	1516	rBV8	4880	7137	1.07%	0.137%
13	6.066	1550	1563	1580	rBV	155525	326788	48.87%	6.285%
14	6.985	1838	1849	1865	rBV	64294	122013	18.25%	2.346%
15	7.313	1940	1951	1972	rBV	285205	525241	78.55%	10.101%
16	7.625	2038	2048	2060	rBV2	37034	68475	10.24%	1.317%
17	8.091	2181	2193	2236	rBV2	205393	552946	82.70%	10.634%
18	8.850	2416	2429	2459	rBV	303896	520543	77.85%	10.011%
19	10.217	2841	2854	2871	rBV	101969	168260	25.16%	3.236%
20	11.249	3162	3175	3194	rBV	272951	427412	63.92%	8.220%
21	11.625	3281	3292	3311	rBV	251706	406973	60.86%	7.827%




Sum of corrected areas: 5199889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027298.D
Acq On : 12 Aug 2022 00:12
Operator : SY/MD
Sample : N4162-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

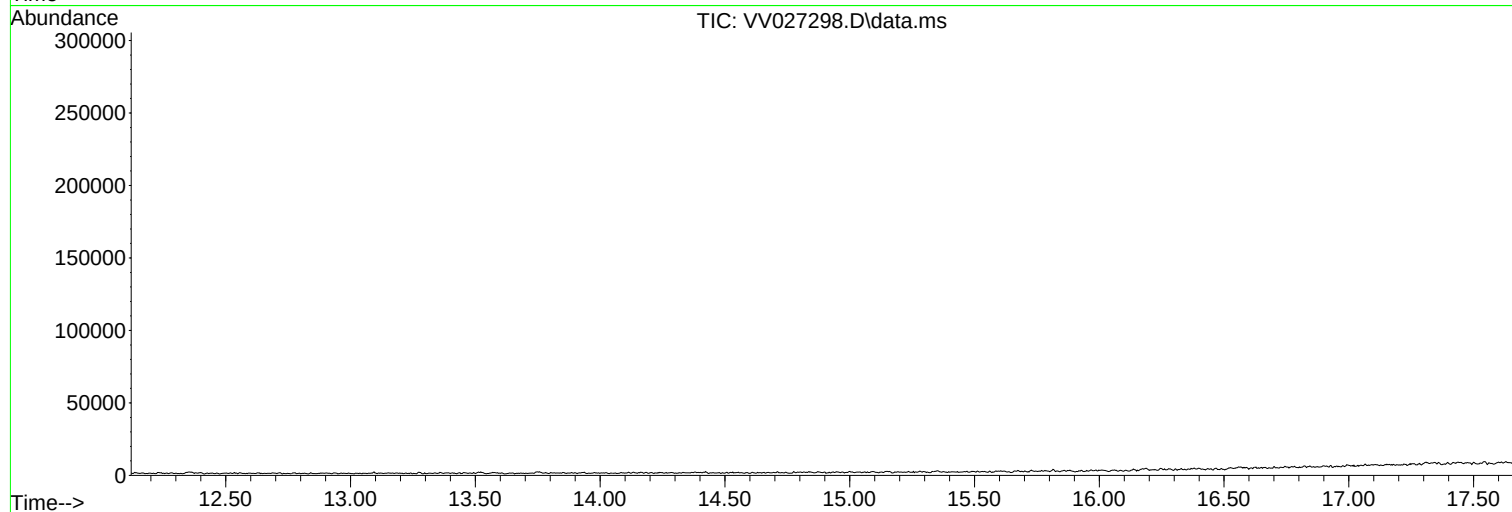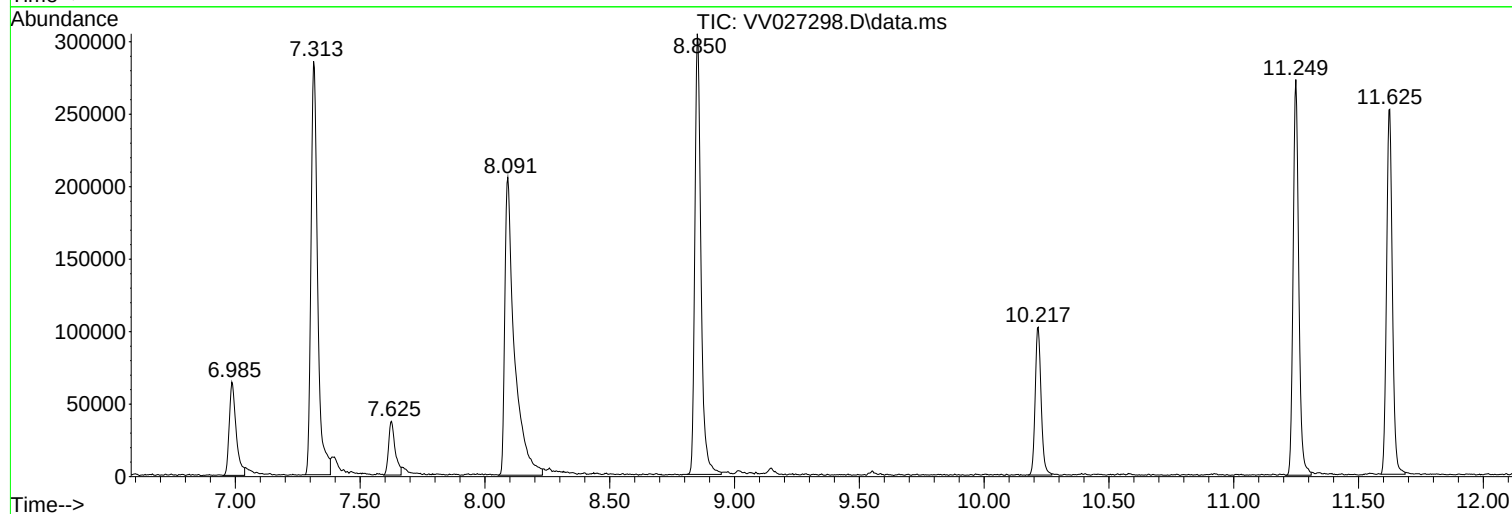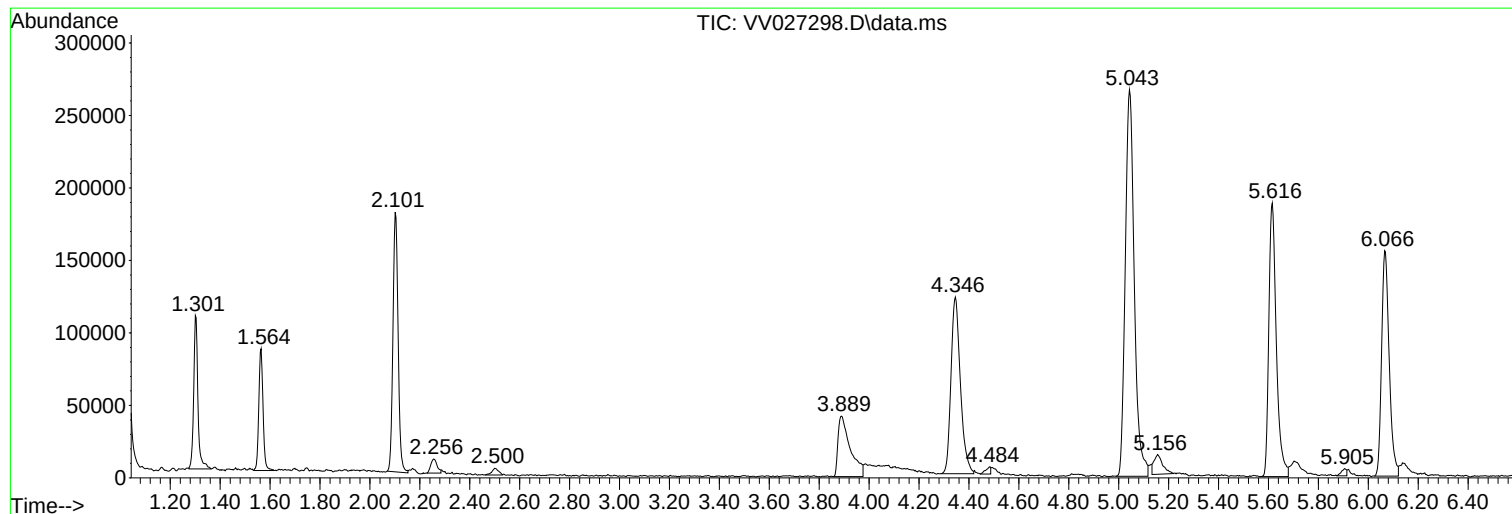

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027298.D
Acq On : 12 Aug 2022 00:12
Operator : SY/MD
Sample : N4162-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027298.D
Acq On : 12 Aug 2022 00:12
Operator : SY/MD
Sample : N4162-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc