

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027299.D
 Acq On : 12 Aug 2022 00:37
 Operator : SY/MD
 Sample : N4162-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBW1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.159	32	37	46	rVB	6703	7503	1.12%	0.145%
2	1.304	74	82	91	rBV	109112	113572	16.92%	2.196%
3	1.564	155	163	173	rBV	84400	97577	14.54%	1.886%
4	2.101	319	330	344	rBV	181754	259515	38.66%	5.017%
5	2.249	368	376	385	rBV	9492	15587	2.32%	0.301%
6	3.889	877	886	911	rBV	40334	136808	20.38%	2.645%
7	4.346	1011	1028	1053	rBV	120354	305298	45.48%	5.902%
8	5.043	1229	1245	1268	rBV3	266417	671267	100.00%	12.977%
9	5.149	1271	1278	1295	rVB4	10980	28567	4.26%	0.552%
10	5.616	1411	1423	1444	rBV	190760	398154	59.31%	7.697%
11	6.066	1550	1563	1582	rBV	158190	332935	49.60%	6.436%
12	6.133	1582	1584	1605	rVB10	8333	15979	2.38%	0.309%
13	6.985	1839	1849	1863	rBV	61881	119329	17.78%	2.307%
14	7.313	1939	1951	1977	rBV	285685	536317	79.90%	10.368%
15	7.625	2039	2048	2065	rBV2	36546	73909	11.01%	1.429%
16	8.091	2182	2193	2237	rBV2	209792	543306	80.94%	10.503%
17	8.850	2418	2429	2454	rBV	303004	517230	77.05%	9.999%
18	10.217	2837	2854	2869	rBV	103310	170936	25.46%	3.304%
19	11.249	3164	3175	3200	rBV	264263	423789	63.13%	8.192%
20	11.622	3278	3291	3310	rBV	249937	405357	60.39%	7.836%




Sum of corrected areas: 5172935

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027299.D
Acq On : 12 Aug 2022 00:37
Operator : SY/MD
Sample : N4162-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

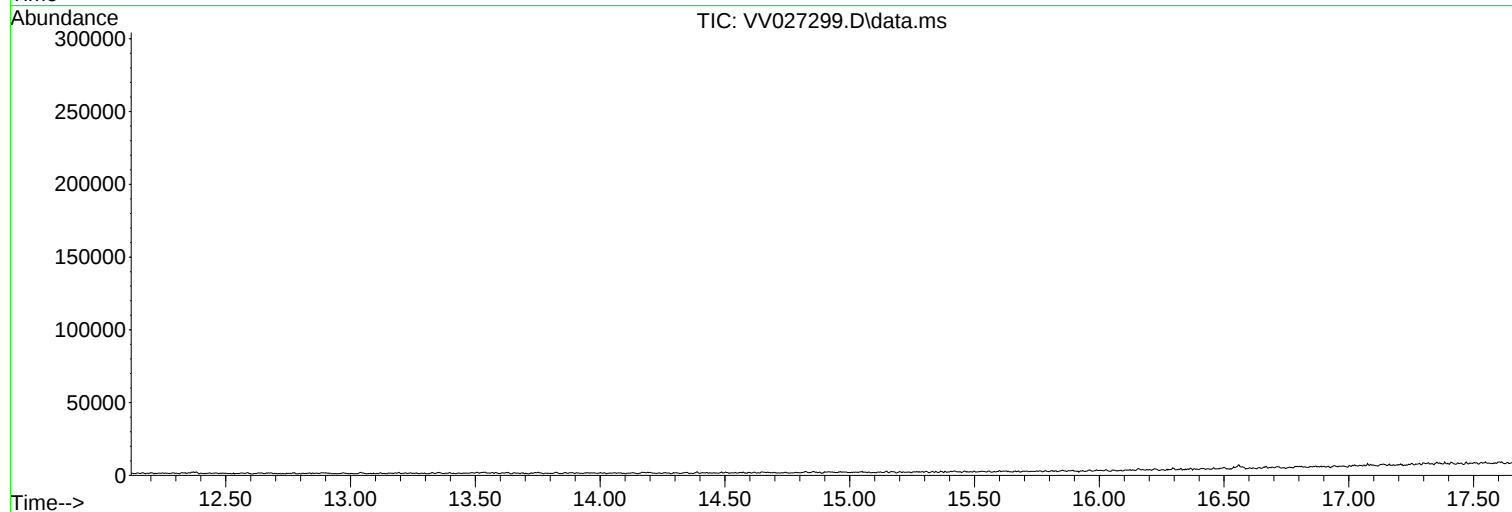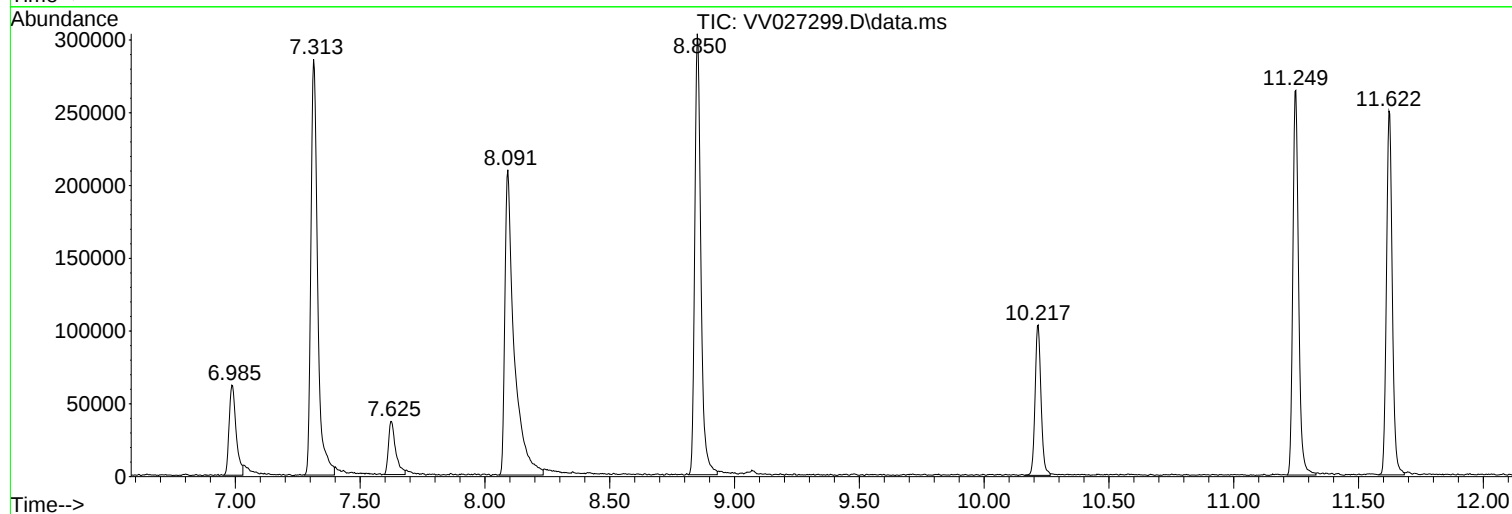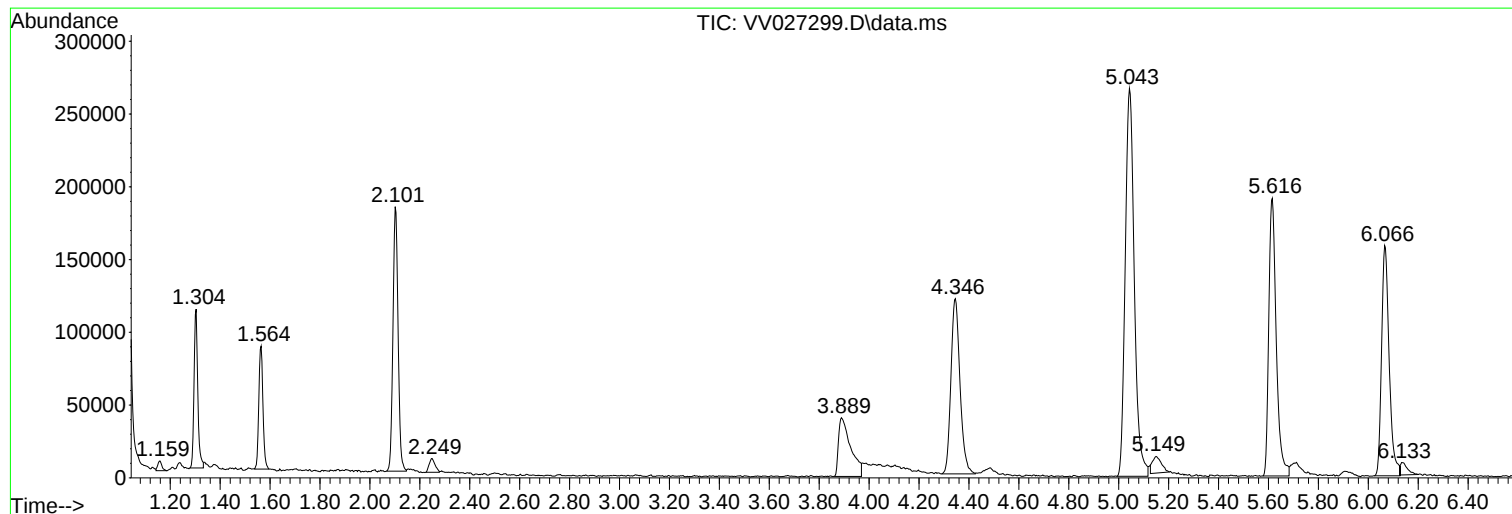

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027299.D
Acq On : 12 Aug 2022 00:37
Operator : SY/MD
Sample : N4162-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027299.D
Acq On : 12 Aug 2022 00:37
Operator : SY/MD
Sample : N4162-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc