

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027300.D
 Acq On : 12 Aug 2022 01:02
 Operator : SY/MD
 Sample : N4162-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBW4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.156	31	36	43	rVB	7647	8201	1.21%	0.156%
2	1.301	74	81	103	rVB	110346	118899	17.49%	2.267%
3	1.561	155	162	178	rVB	87186	101325	14.90%	1.932%
4	2.101	319	330	344	rBV	183717	263380	38.74%	5.021%
5	2.246	367	375	383	rBV	9325	15516	2.28%	0.296%
6	3.889	875	886	905	rBV2	43647	134657	19.81%	2.567%
7	4.342	1011	1027	1054	rBV	120877	310955	45.74%	5.928%
8	4.481	1062	1070	1085	rVB3	5559	12909	1.90%	0.246%
9	5.043	1227	1245	1268	rBV2	271534	679888	100.00%	12.961%
10	5.149	1272	1278	1299	rVB4	11733	31922	4.70%	0.609%
11	5.612	1411	1422	1443	rBV	189302	395282	58.14%	7.535%
12	5.702	1444	1450	1468	rVB2	9016	23226	3.42%	0.443%
13	6.066	1549	1563	1581	rBV2	158825	336660	49.52%	6.418%
14	6.985	1840	1849	1867	rBV	63669	123857	18.22%	2.361%
15	7.313	1939	1951	1984	rBV	295984	547672	80.55%	10.441%
16	7.622	2036	2047	2065	rBV2	36559	73979	10.88%	1.410%
17	8.091	2180	2193	2234	rBV	218161	556939	81.92%	10.617%
18	8.850	2418	2429	2454	rBV	298066	513639	75.55%	9.792%
19	10.217	2842	2854	2871	rBV	104574	171514	25.23%	3.270%
20	11.249	3164	3175	3193	rBV	259744	416830	61.31%	7.946%
21	11.622	3280	3291	3315	rBV	255465	408358	60.06%	7.785%




Sum of corrected areas: 5245608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027300.D
Acq On : 12 Aug 2022 01:02
Operator : SY/MD
Sample : N4162-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

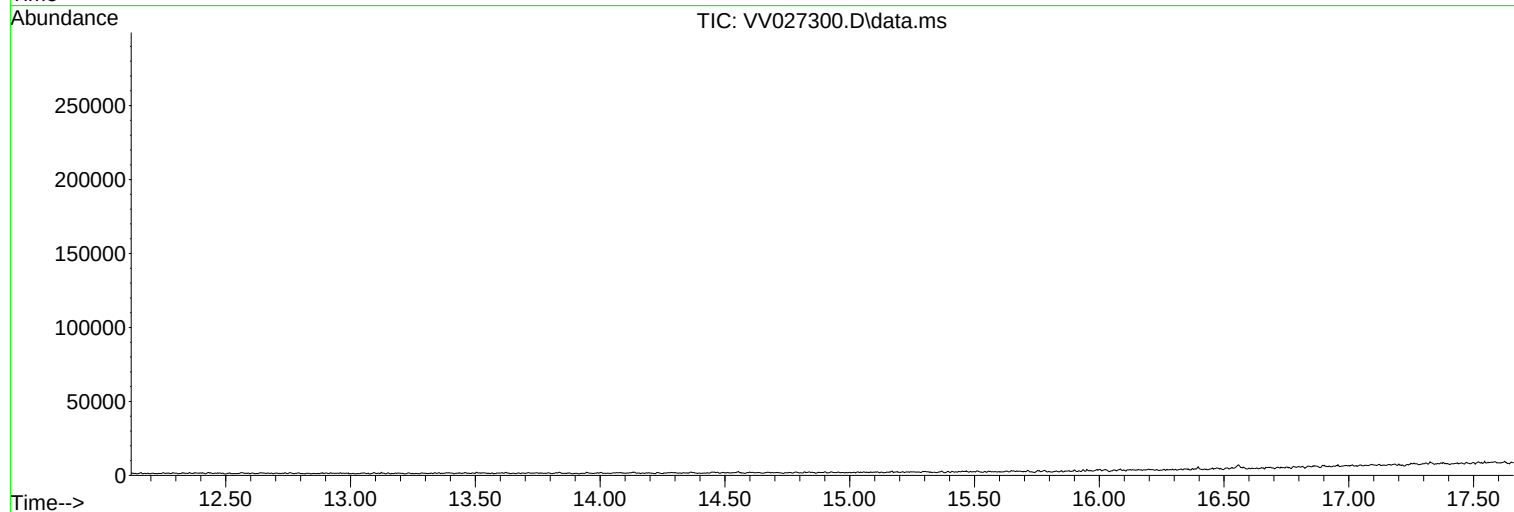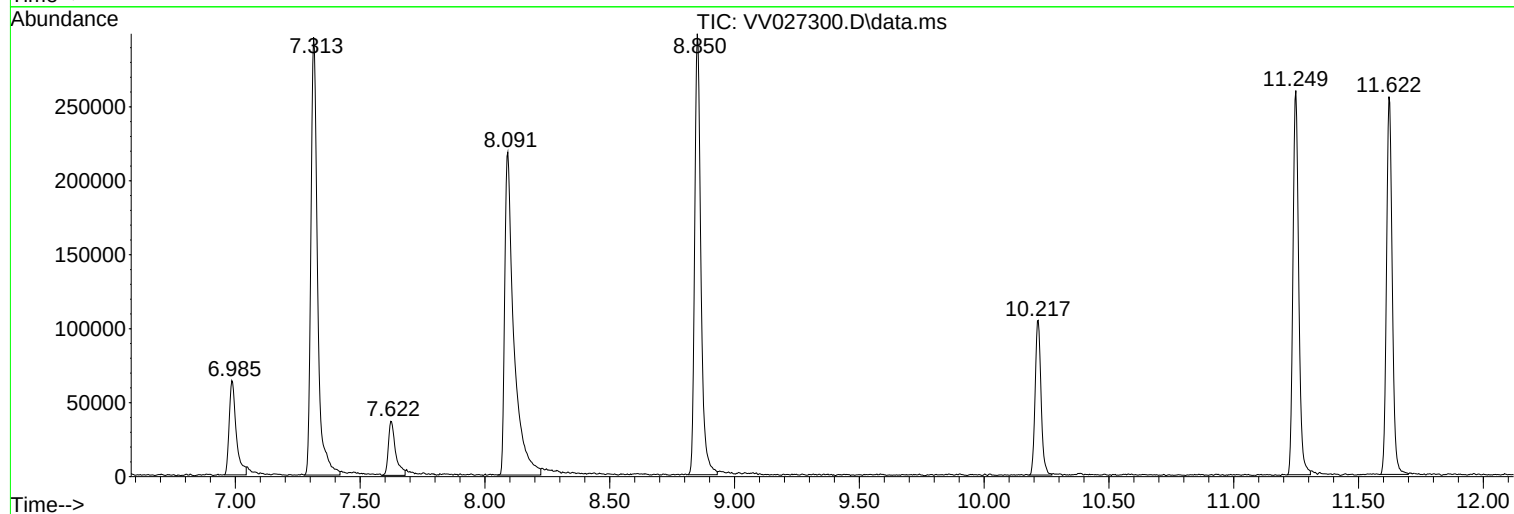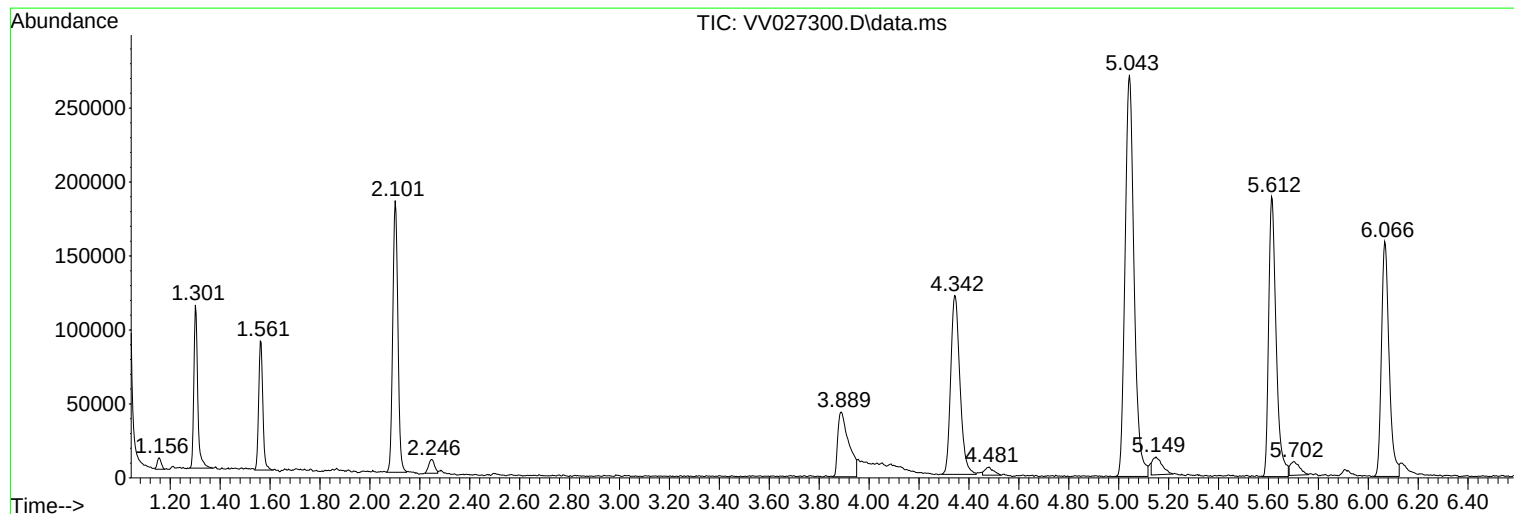

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027300.D
Acq On : 12 Aug 2022 01:02
Operator : SY/MD
Sample : N4162-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027300.D
Acq On : 12 Aug 2022 01:02
Operator : SY/MD
Sample : N4162-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc