

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027301.D
 Acq On : 12 Aug 2022 01:27
 Operator : SY/MD
 Sample : N4162-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	20	24	29	rBV	5828	6957	1.04%	0.133%
2	1.143	29	32	43	rVB	9232	10399	1.56%	0.199%
3	1.304	75	82	96	rBV	106418	114055	17.07%	2.186%
4	1.564	153	163	173	rBV	84506	100513	15.04%	1.927%
5	2.101	319	330	344	rBV	176756	254457	38.07%	4.878%
6	2.236	362	372	384	rBV2	8884	17447	2.61%	0.334%
7	3.886	875	885	912	rBV2	46508	164273	24.58%	3.149%
8	4.342	1011	1027	1056	rBV	121838	326007	48.78%	6.250%
9	4.474	1056	1068	1080	rVB4	4248	11584	1.73%	0.222%
10	5.043	1229	1245	1268	rBV2	265139	668338	100.00%	12.812%
11	5.612	1410	1422	1442	rBV	186011	393232	58.84%	7.538%
12	5.912	1505	1515	1530	rBV	7828	18372	2.75%	0.352%
13	6.066	1551	1563	1579	rBV	156667	326413	48.84%	6.257%
14	6.985	1838	1849	1872	rBV	61057	124830	18.68%	2.393%
15	7.313	1938	1951	1983	rBV	286908	537132	80.37%	10.297%
16	7.622	2037	2047	2063	rBV2	36802	71296	10.67%	1.367%
17	8.091	2180	2193	2230	rBV2	237070	556531	83.27%	10.669%
18	8.850	2416	2429	2453	rBV	300611	517566	77.44%	9.922%
19	10.214	2843	2853	2872	rBV2	100886	166761	24.95%	3.197%
20	11.249	3164	3175	3195	rBV	262835	421327	63.04%	8.077%
21	11.622	3278	3291	3309	rBV	255607	408901	61.18%	7.839%




Sum of corrected areas: 5216391

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027301.D
Acq On : 12 Aug 2022 01:27
Operator : SY/MD
Sample : N4162-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

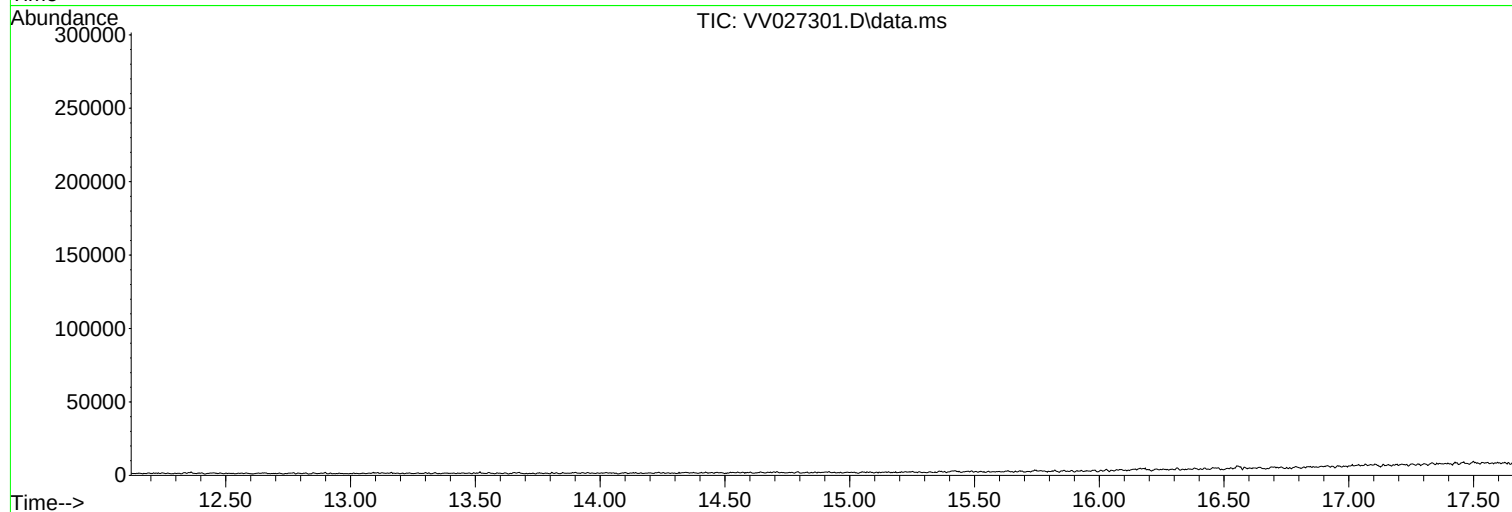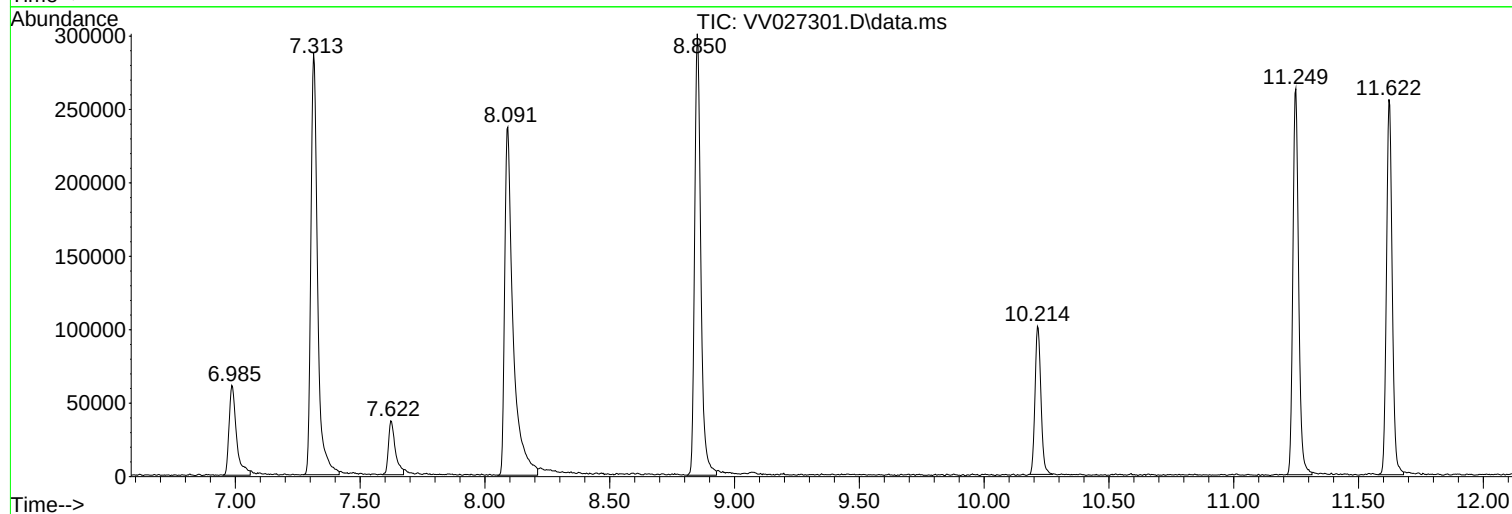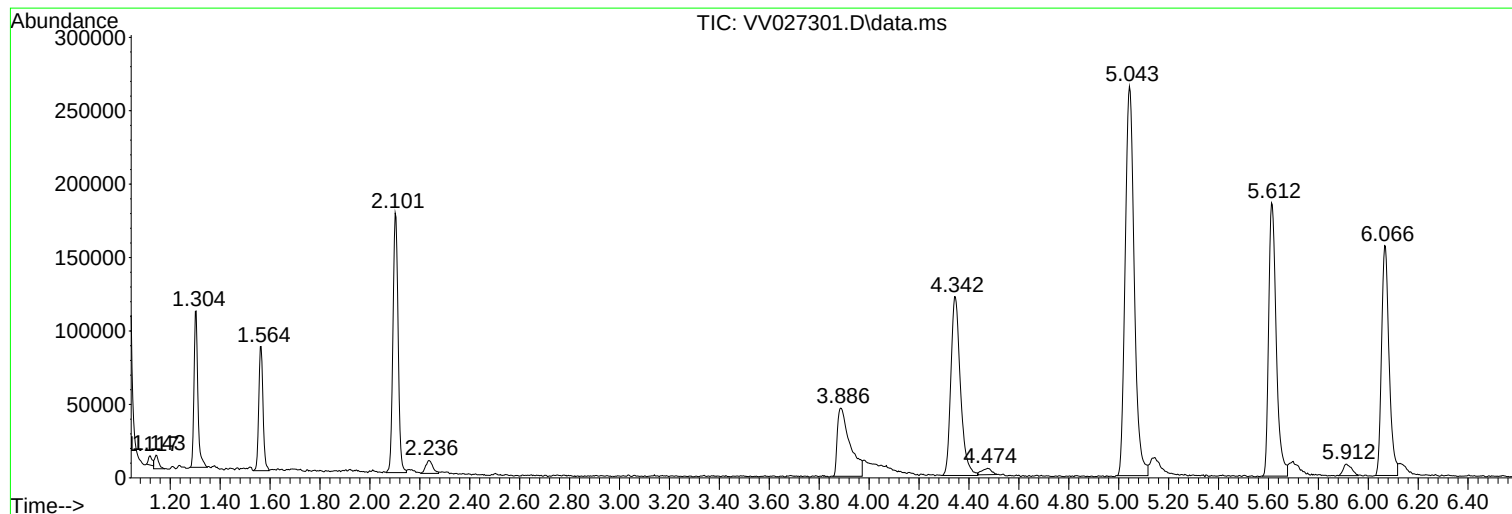

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027301.D
Acq On : 12 Aug 2022 01:27
Operator : SY/MD
Sample : N4162-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027301.D
Acq On : 12 Aug 2022 01:27
Operator : SY/MD
Sample : N4162-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc