

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027302.D
 Acq On : 12 Aug 2022 01:52
 Operator : SY/MD
 Sample : N4162-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	27	rVV2	8283	8538	1.28%	0.159%
2	1.146	28	33	42	rVB	12918	14990	2.25%	0.280%
3	1.301	74	81	95	rBV	106439	118161	17.77%	2.205%
4	1.564	155	163	173	rBV	84301	98747	14.85%	1.843%
5	2.101	321	330	349	rVB	178657	256388	38.57%	4.785%
6	2.233	363	371	384	rVB2	9851	17359	2.61%	0.324%
7	3.886	874	885	918	rBV2	62151	216664	32.59%	4.044%
8	4.346	1008	1028	1053	rBV	119108	315091	47.40%	5.881%
9	5.043	1228	1245	1266	rBV2	263246	664781	100.00%	12.408%
10	5.143	1269	1276	1290	rVB4	10332	26011	3.91%	0.485%
11	5.612	1410	1422	1443	rBV	190160	396693	59.67%	7.404%
12	5.915	1502	1516	1534	rBV4	46593	104027	15.65%	1.942%
13	6.066	1549	1563	1579	rBV2	157881	328651	49.44%	6.134%
14	6.985	1837	1849	1872	rBV	63060	127240	19.14%	2.375%
15	7.313	1940	1951	1987	rBV	283045	534006	80.33%	9.967%
16	7.622	2038	2047	2073	rBV2	36909	76078	11.44%	1.420%
17	8.088	2180	2192	2221	rBV	246325	535234	80.51%	9.990%
18	8.850	2418	2429	2456	rBV	302745	524143	78.84%	9.783%
19	10.214	2842	2853	2873	rBV	102342	167010	25.12%	3.117%
20	11.249	3161	3175	3196	rBV	264186	424994	63.93%	7.933%
21	11.622	3280	3291	3310	rBV	252397	402808	60.59%	7.518%




Sum of corrected areas: 5357614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027302.D
Acq On : 12 Aug 2022 01:52
Operator : SY/MD
Sample : N4162-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

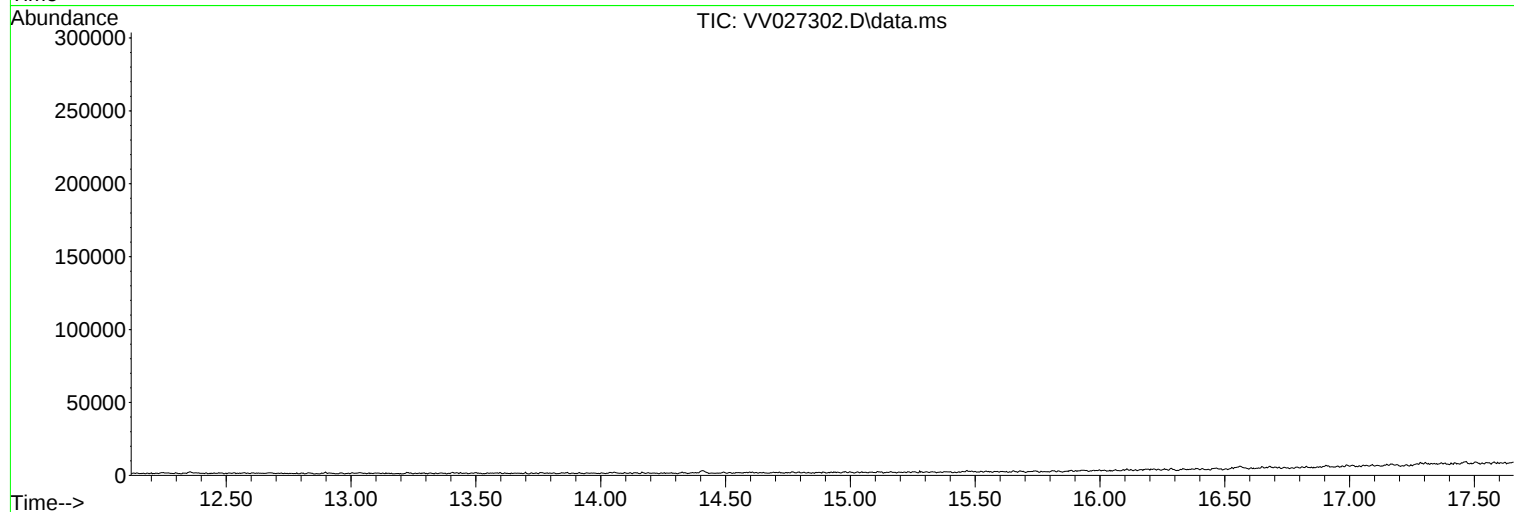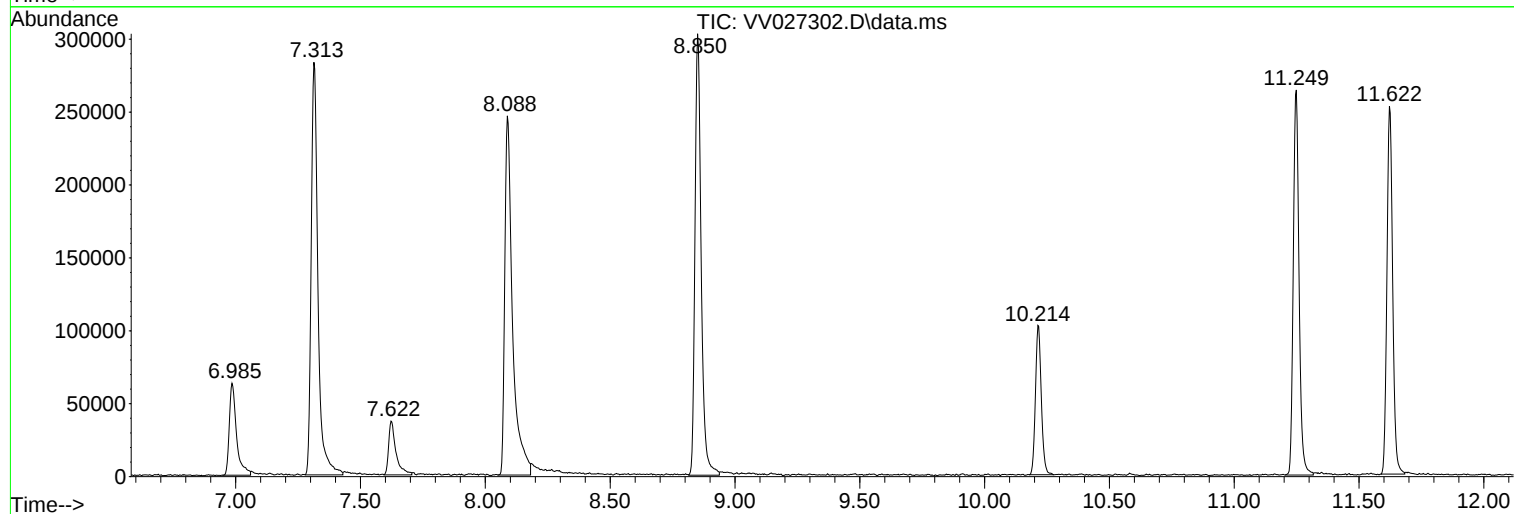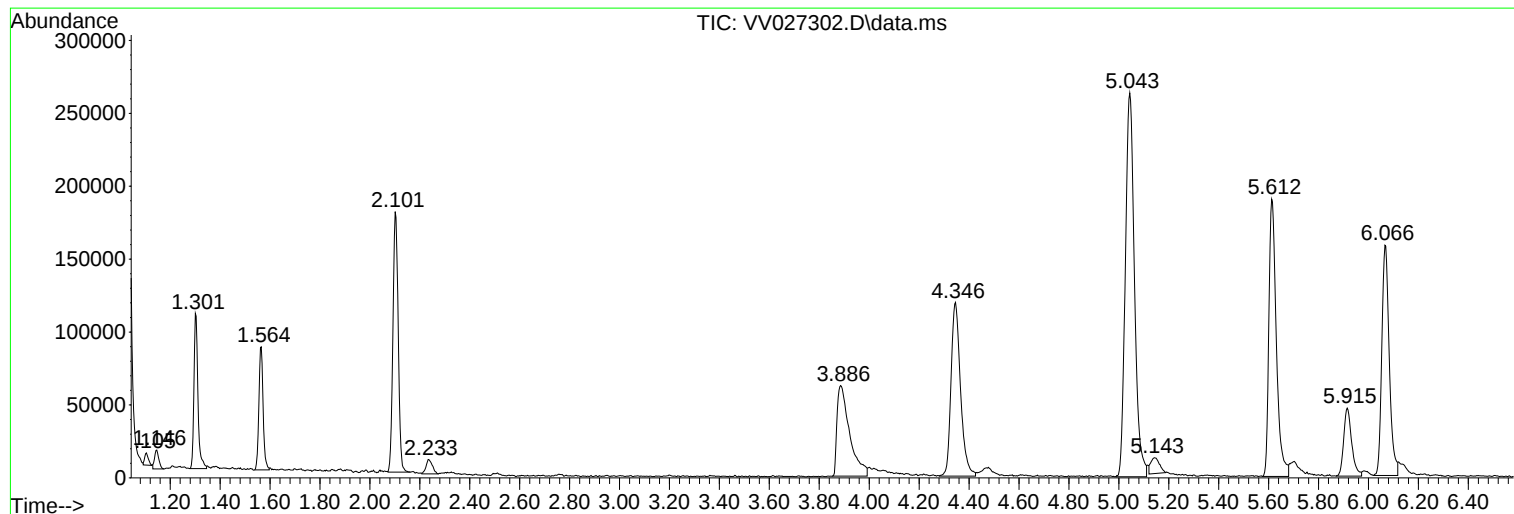

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027302.D
Acq On : 12 Aug 2022 01:52
Operator : SY/MD
Sample : N4162-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027302.D
Acq On : 12 Aug 2022 01:52
Operator : SY/MD
Sample : N4162-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc