

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027304.D
 Acq On : 12 Aug 2022 02:42
 Operator : SY/MD
 Sample : N4162-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBY0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.140	26	31	43	rVB	13603	17684	2.68%	0.329%
2	1.304	75	82	101	rVB	106728	118682	17.98%	2.208%
3	1.564	155	163	176	rVB	88893	98792	14.97%	1.838%
4	2.101	320	330	346	rBV	179345	258547	39.18%	4.809%
5	2.233	361	371	379	rBV3	9637	16654	2.52%	0.310%
6	3.892	875	887	909	rBV3	48706	176565	26.76%	3.284%
7	4.346	1011	1028	1051	rBV2	120168	317618	48.13%	5.908%
8	5.043	1230	1245	1267	rBV2	263953	659906	100.00%	12.276%
9	5.143	1268	1276	1290	rVB5	11207	28329	4.29%	0.527%
10	5.612	1411	1422	1441	rBV	191102	395713	59.97%	7.361%
11	5.915	1504	1516	1533	rBV2	80539	171262	25.95%	3.186%
12	6.066	1550	1563	1581	rBV	157178	330379	50.06%	6.146%
13	6.985	1832	1849	1877	rBV	61798	130232	19.73%	2.423%
14	7.313	1938	1951	1983	rBV	287025	534338	80.97%	9.940%
15	7.625	2038	2048	2066	rBV2	36306	72751	11.02%	1.353%
16	8.091	2179	2193	2224	rBV	221864	536277	81.27%	9.976%
17	8.850	2416	2429	2449	rBV	301788	515919	78.18%	9.597%
18	10.217	2842	2854	2873	rBV	102545	170212	25.79%	3.166%
19	11.249	3164	3175	3196	rBV	262450	421558	63.88%	7.842%
20	11.622	3280	3291	3313	rBV	249008	404370	61.28%	7.522%




Sum of corrected areas: 5375788

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027304.D
Acq On : 12 Aug 2022 02:42
Operator : SY/MD
Sample : N4162-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

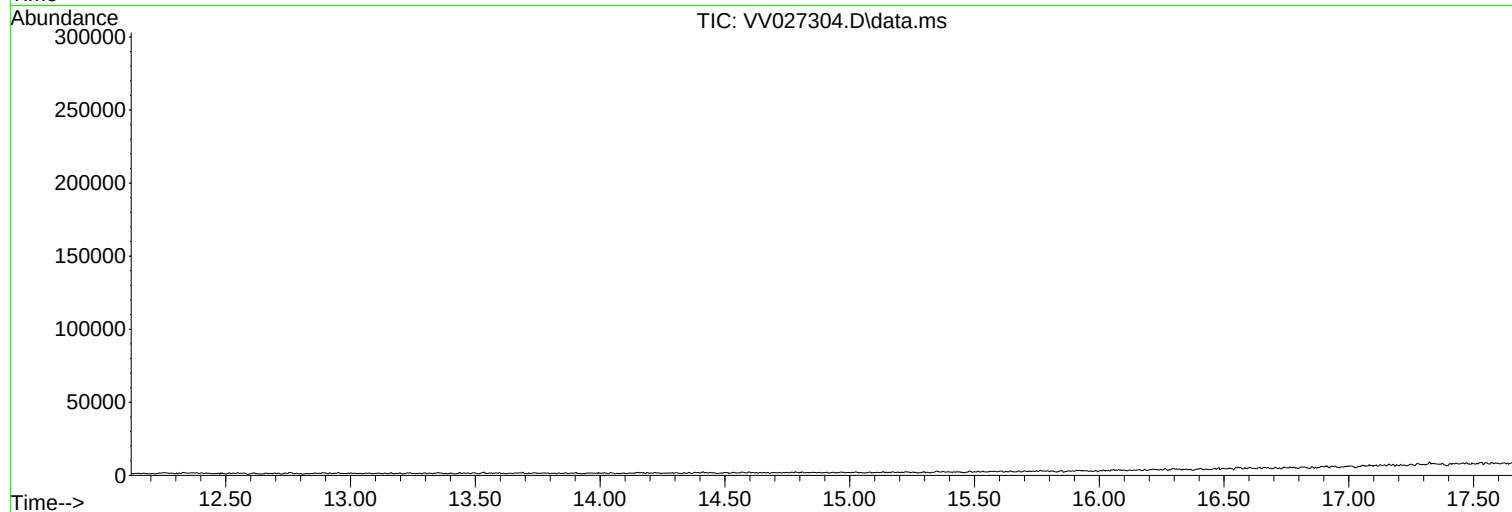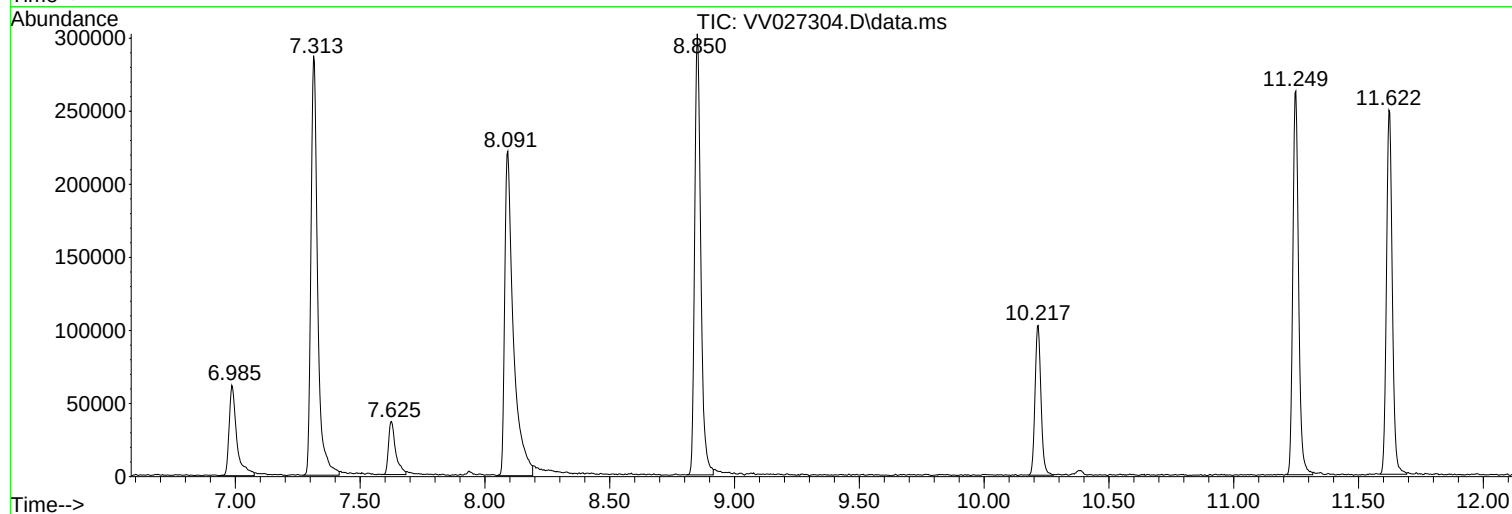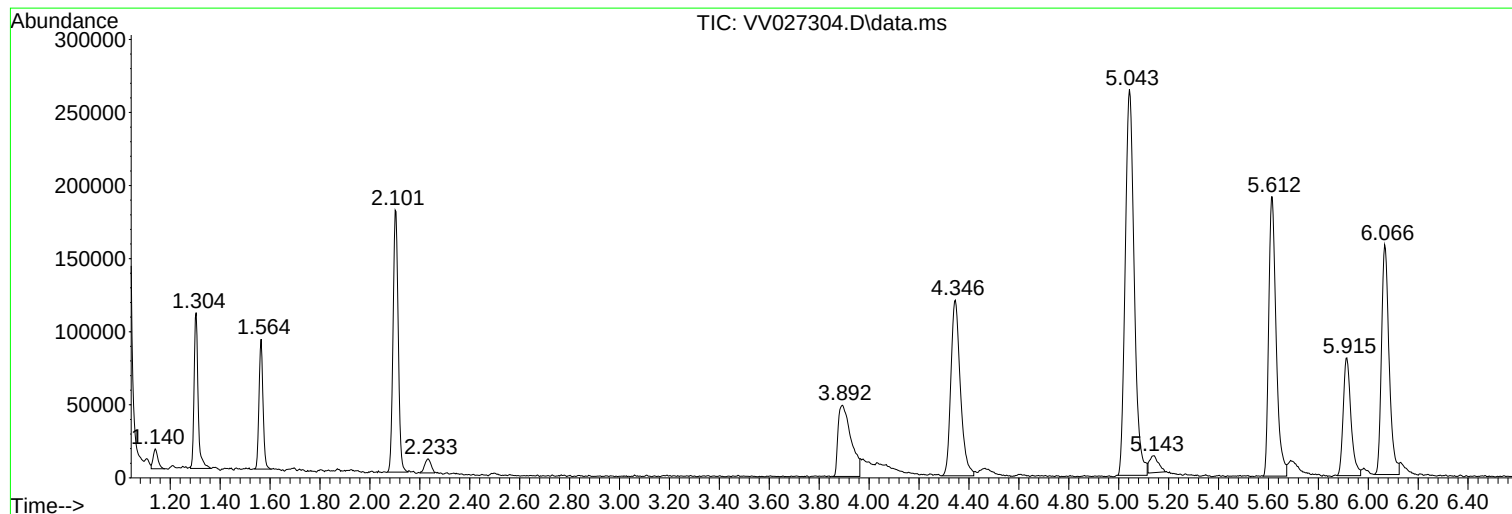

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027304.D
Acq On : 12 Aug 2022 02:42
Operator : SY/MD
Sample : N4162-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027304.D
Acq On : 12 Aug 2022 02:42
Operator : SY/MD
Sample : N4162-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc