

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027305.D
 Acq On : 12 Aug 2022 03:07
 Operator : SY/MD
 Sample : N4162-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBY1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	40	rVB	12056	16569	2.46%	0.304%
2	1.304	75	82	99	rVB	110737	120050	17.84%	2.206%
3	1.565	154	163	175	rBV	86149	100105	14.87%	1.839%
4	2.101	320	330	346	rBV	182480	262600	39.02%	4.824%
5	2.224	360	368	382	rVB2	9036	17996	2.67%	0.331%
6	3.892	875	887	908	rBV	50422	174584	25.94%	3.207%
7	4.343	1012	1027	1053	rBV	120503	309397	45.97%	5.684%
8	5.043	1227	1245	1265	rBV2	270373	673070	100.00%	12.365%
9	5.613	1410	1422	1440	rBV	194030	399846	59.41%	7.346%
10	5.687	1442	1445	1459	rVB2	9001	17986	2.67%	0.330%
11	5.912	1502	1515	1531	rBV	91555	191394	28.44%	3.516%
12	6.066	1550	1563	1583	rBV	160024	333279	49.52%	6.123%
13	6.986	1837	1849	1872	rBV2	61476	124873	18.55%	2.294%
14	7.313	1940	1951	1983	rBV	294180	540902	80.36%	9.937%
15	7.622	2033	2047	2062	rBV2	36530	70216	10.43%	1.290%
16	8.092	2181	2193	2223	rBV	223288	545449	81.04%	10.021%
17	8.850	2418	2429	2452	rBV	308911	531417	78.95%	9.763%
18	10.217	2842	2854	2867	rBV	102436	168821	25.08%	3.102%
19	11.249	3161	3175	3196	rBV	268656	429557	63.82%	7.892%
20	11.622	3280	3291	3310	rBV	254213	415041	61.66%	7.625%




Sum of corrected areas: 5443152

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027305.D
Acq On : 12 Aug 2022 03:07
Operator : SY/MD
Sample : N4162-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

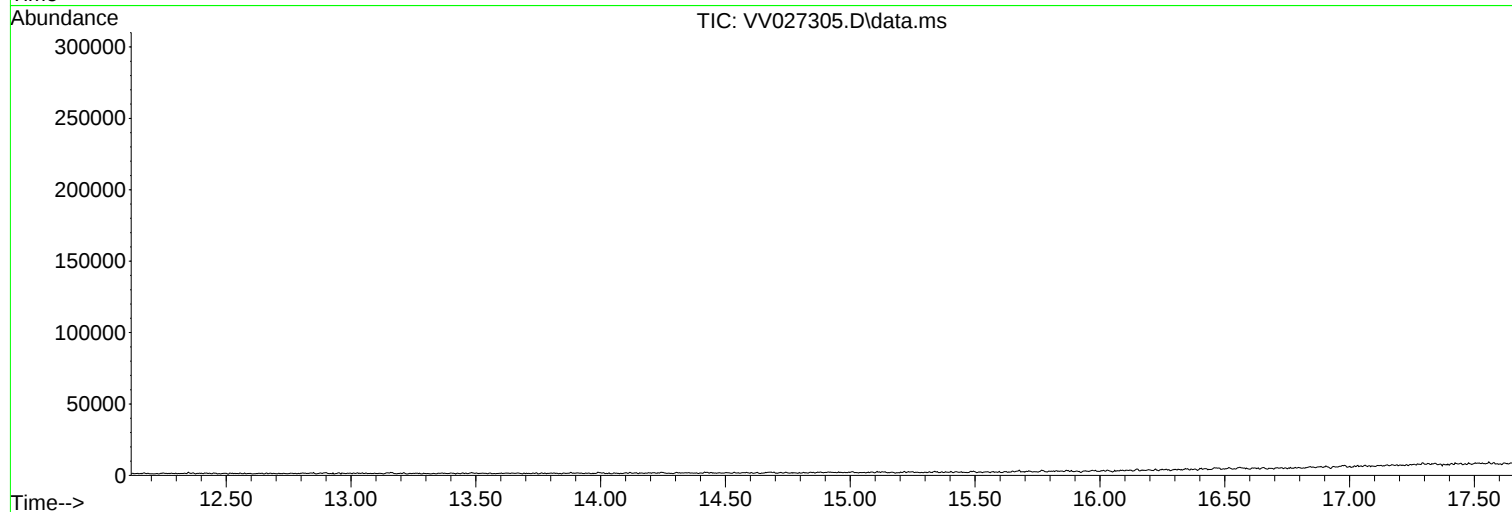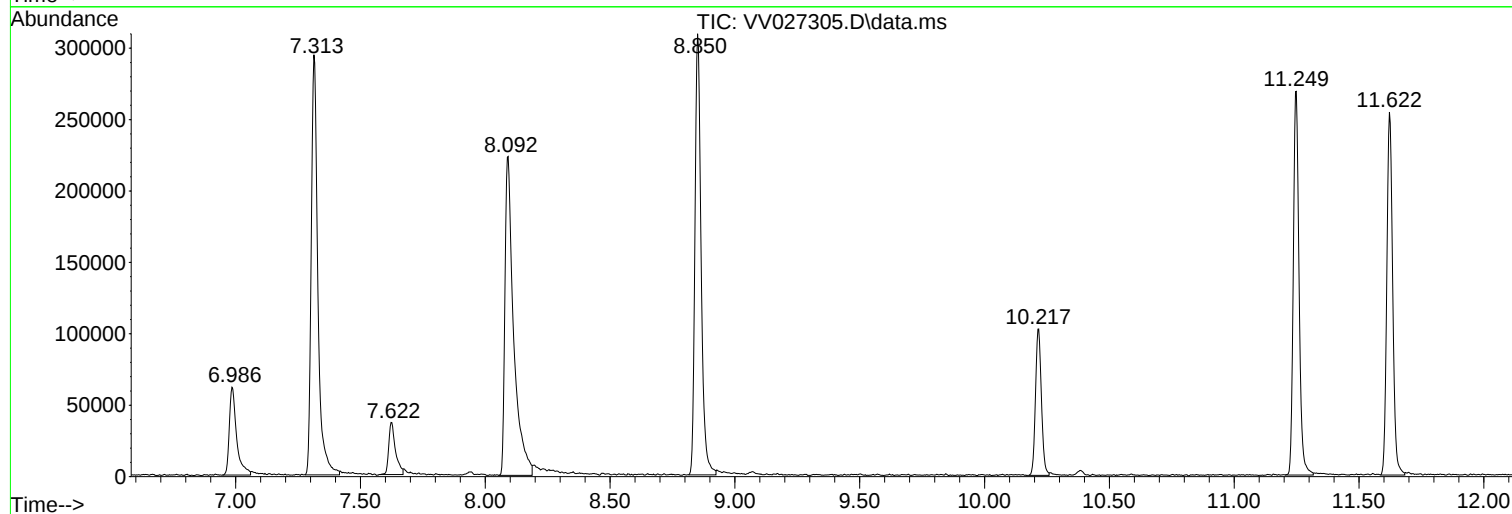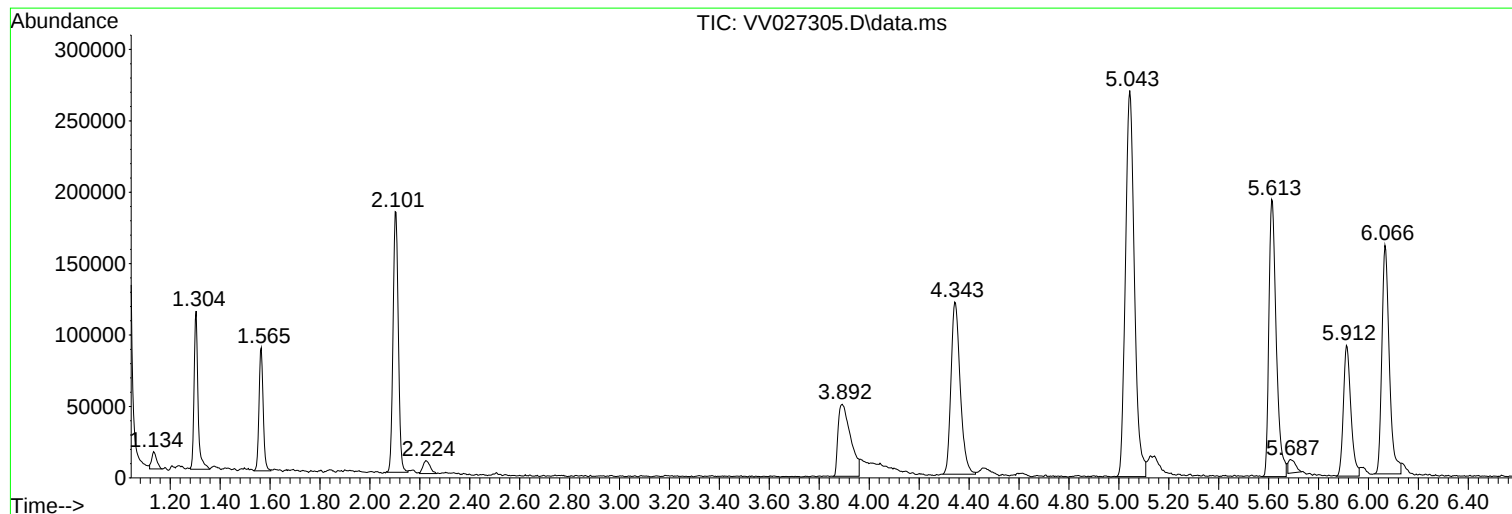

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027305.D
Acq On : 12 Aug 2022 03:07
Operator : SY/MD
Sample : N4162-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027305.D
Acq On : 12 Aug 2022 03:07
Operator : SY/MD
Sample : N4162-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
