

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027307.D
 Acq On : 12 Aug 2022 03:57
 Operator : SY/MD
 Sample : N4162-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBY3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	22	27	37	rVB2	14011	18958	1.81%	0.291%
2	1.301	75	81	95	rBV	107652	115197	11.00%	1.770%
3	1.561	154	162	173	rVB	87946	100124	9.56%	1.538%
4	2.101	320	330	342	rBV	178576	256020	24.44%	3.934%
5	2.217	356	366	380	rBV3	8384	16996	1.62%	0.261%
6	3.899	868	889	919	rBV4	113502	429257	40.98%	6.595%
7	4.342	1011	1027	1051	rBV	121110	309117	29.51%	4.749%
8	4.458	1057	1063	1079	rVB6	4899	11365	1.09%	0.175%
9	4.603	1093	1108	1127	rVB2	24671	64003	6.11%	0.983%
10	5.043	1228	1245	1264	rBV2	265840	666846	63.67%	10.246%
11	5.613	1409	1422	1440	rBV	186477	389078	37.15%	5.978%
12	5.908	1501	1514	1530	rBV	531053	1047414	100.00%	16.093%
13	6.066	1551	1563	1598	rVB	160006	349248	33.34%	5.366%
14	6.985	1838	1849	1873	rBV	62795	124867	11.92%	1.918%
15	7.313	1940	1951	1971	rBV	291169	531265	50.72%	8.162%
16	7.622	2037	2047	2069	rBV2	34861	72429	6.92%	1.113%
17	8.088	2181	2192	2220	rBV	249643	522662	49.90%	8.030%
18	8.850	2416	2429	2451	rBV	299780	508206	48.52%	7.808%
19	10.214	2841	2853	2867	rBV	100585	163617	15.62%	2.514%
20	11.249	3163	3175	3191	rBV	255030	413752	39.50%	6.357%
21	11.622	3279	3291	3310	rBV	247002	398248	38.02%	6.119%




Sum of corrected areas: 6508669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027307.D
Acq On : 12 Aug 2022 03:57
Operator : SY/MD
Sample : N4162-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

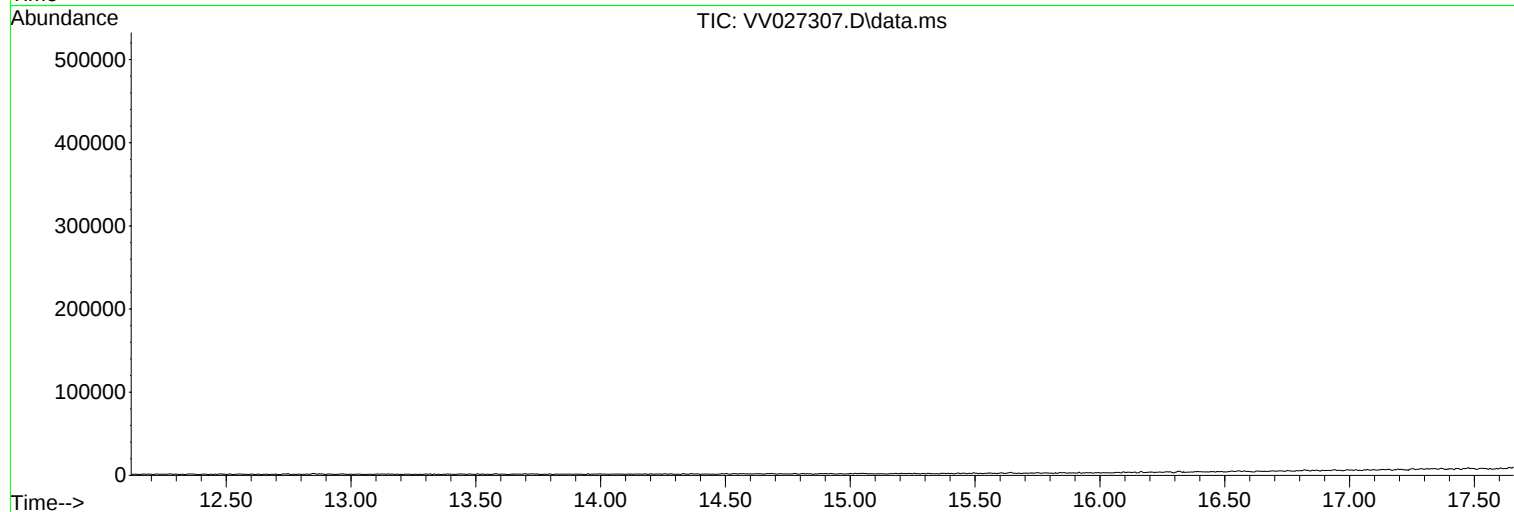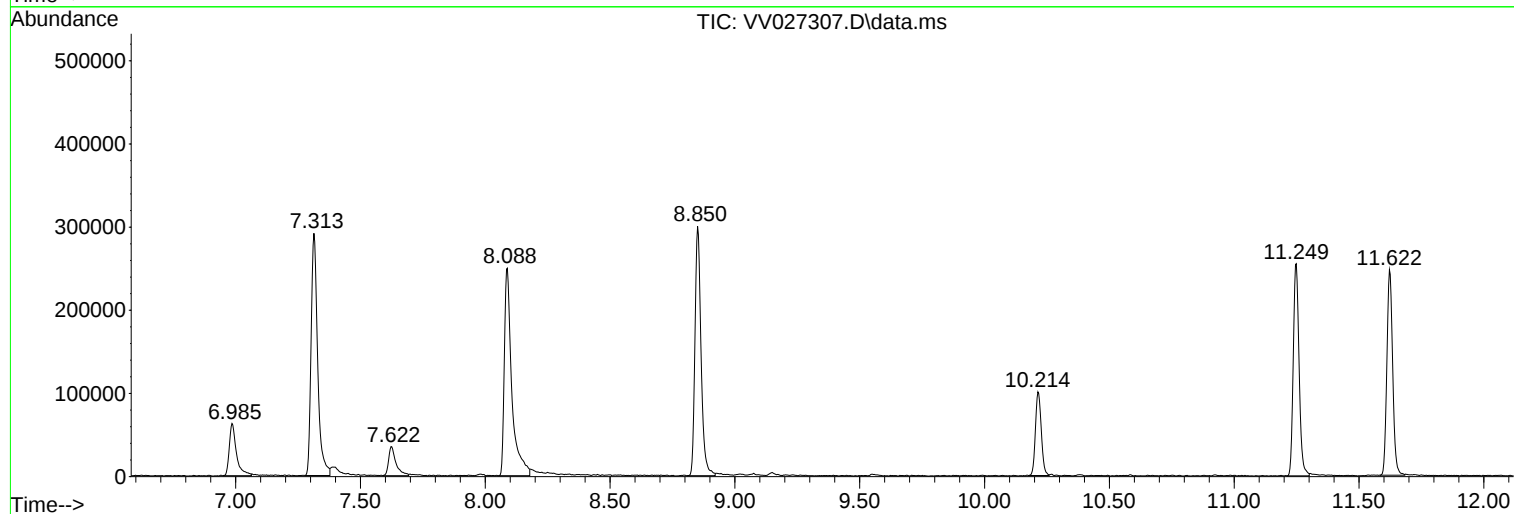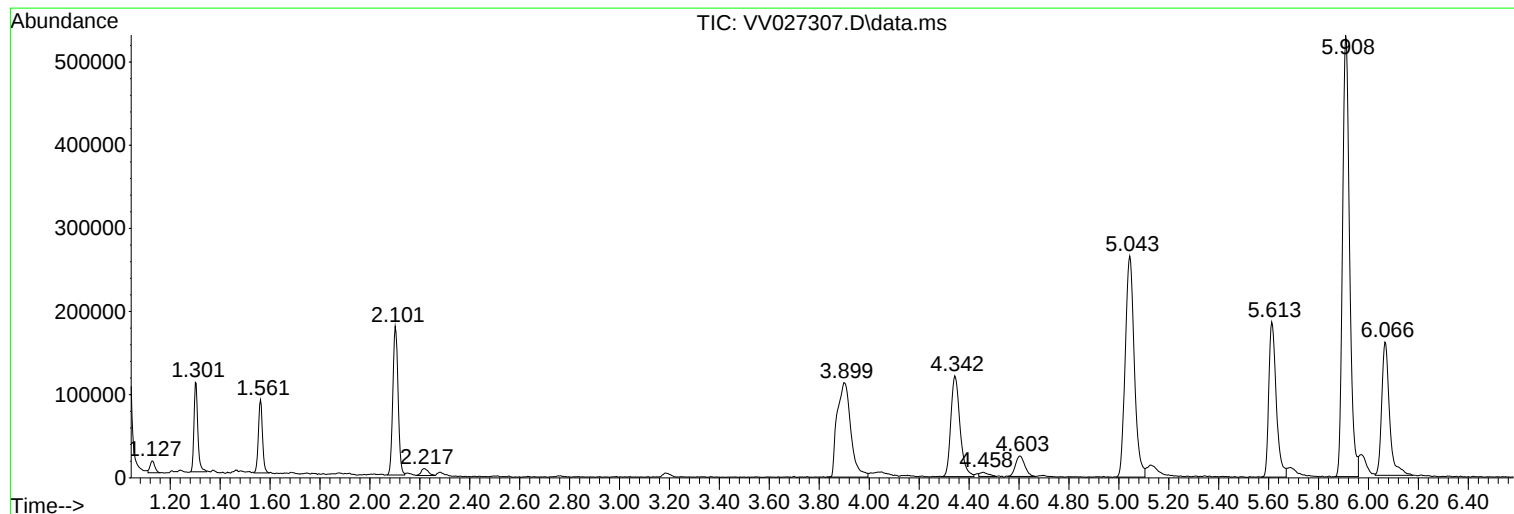

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027307.D
Acq On : 12 Aug 2022 03:57
Operator : SY/MD
Sample : N4162-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027307.D
Acq On : 12 Aug 2022 03:57
Operator : SY/MD
Sample : N4162-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBY3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
