

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027308.D
 Acq On : 12 Aug 2022 04:21
 Operator : SY/MD
 Sample : N4162-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBW9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	19	25	37	rVB	12869	19381	2.94%	0.373%
2	1.304	74	82	99	rVB	109222	117490	17.84%	2.259%
3	1.561	154	162	174	rVB	87077	102726	15.59%	1.975%
4	2.102	317	330	341	rBV	179316	258441	39.23%	4.970%
5	2.211	355	364	376	rBV3	7417	14916	2.26%	0.287%
6	2.285	378	387	401	rVB3	16807	31237	4.74%	0.601%
7	3.873	872	881	914	rBV2	71507	203237	30.85%	3.908%
8	4.346	1010	1028	1050	rBV	124361	322056	48.89%	6.193%
9	4.455	1053	1062	1073	rVB5	3505	9128	1.39%	0.176%
10	5.043	1229	1245	1264	rBV2	263718	658718	100.00%	12.667%
11	5.613	1410	1422	1440	rBV	184570	378966	57.53%	7.287%
12	5.908	1503	1514	1515	rBV9	7001	7354	1.12%	0.141%
13	6.066	1549	1563	1595	rBV	159699	348375	52.89%	6.699%
14	6.986	1838	1849	1864	rBV	60750	118830	18.04%	2.285%
15	7.314	1939	1951	1976	rBV	285920	528940	80.30%	10.171%
16	7.622	2035	2047	2075	rBV2	34919	73375	11.14%	1.411%
17	8.088	2182	2192	2229	rBV	247556	524191	79.58%	10.080%
18	8.850	2418	2429	2452	rBV	293969	500253	75.94%	9.620%
19	10.214	2841	2853	2875	rBV2	101248	168163	25.53%	3.234%
20	11.246	3162	3174	3199	rBV	252780	410318	62.29%	7.890%
21	11.622	3279	3291	3314	rBV	249276	404269	61.37%	7.774%




Sum of corrected areas: 5200364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027308.D
Acq On : 12 Aug 2022 04:21
Operator : SY/MD
Sample : N4162-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

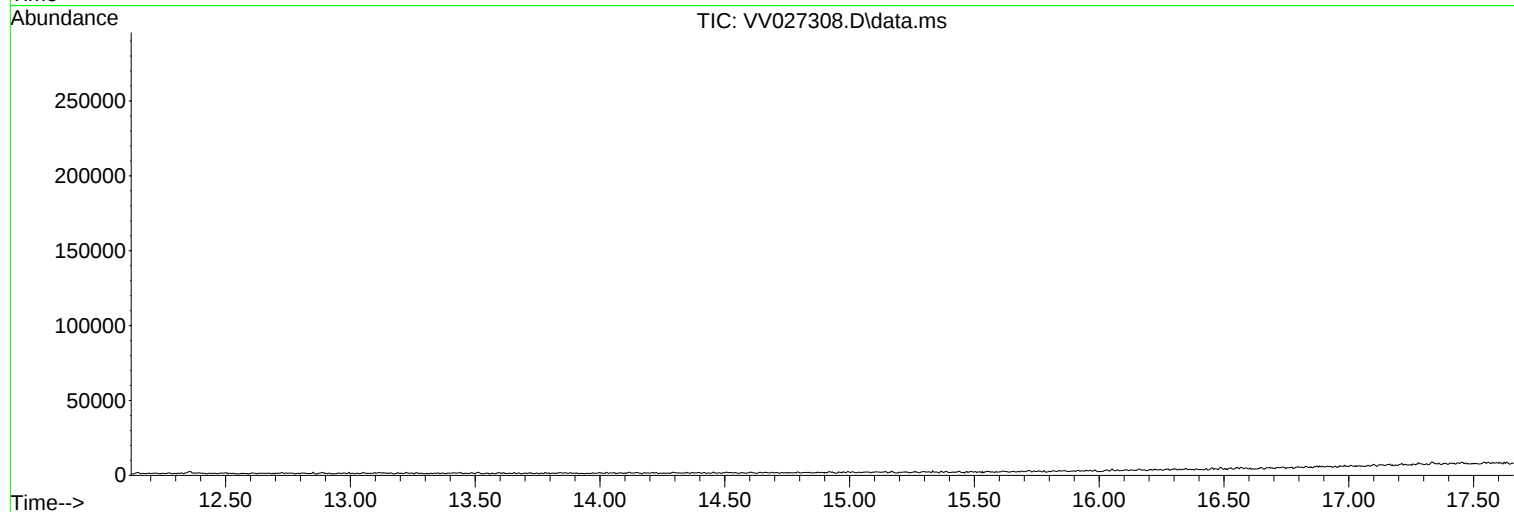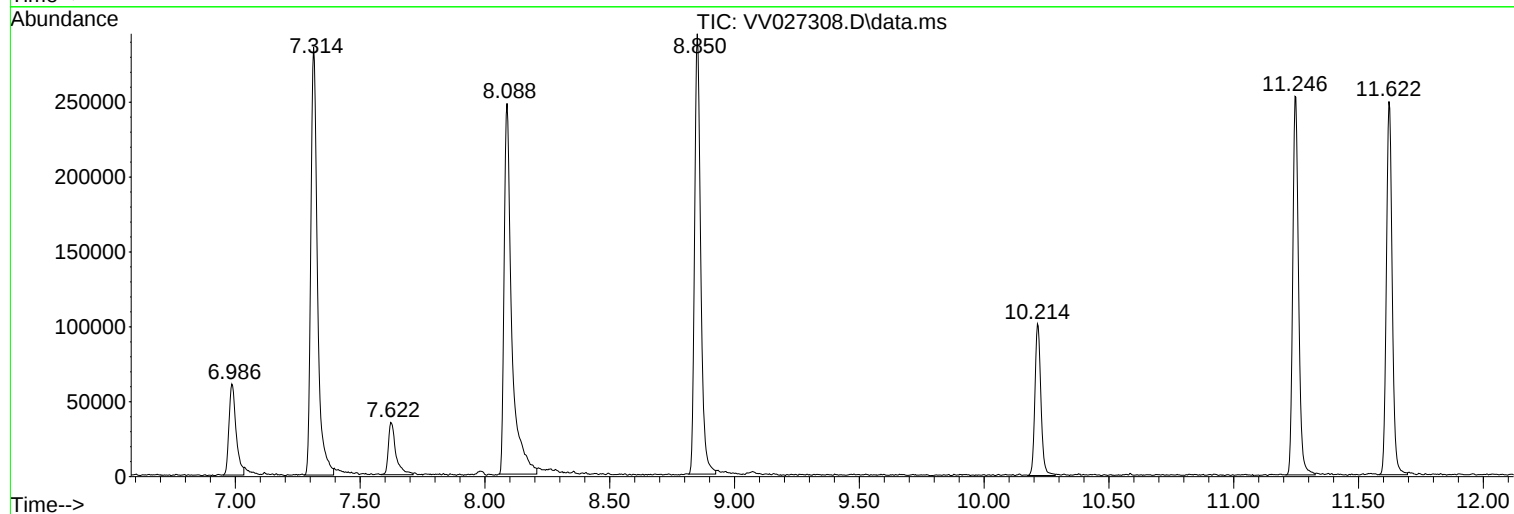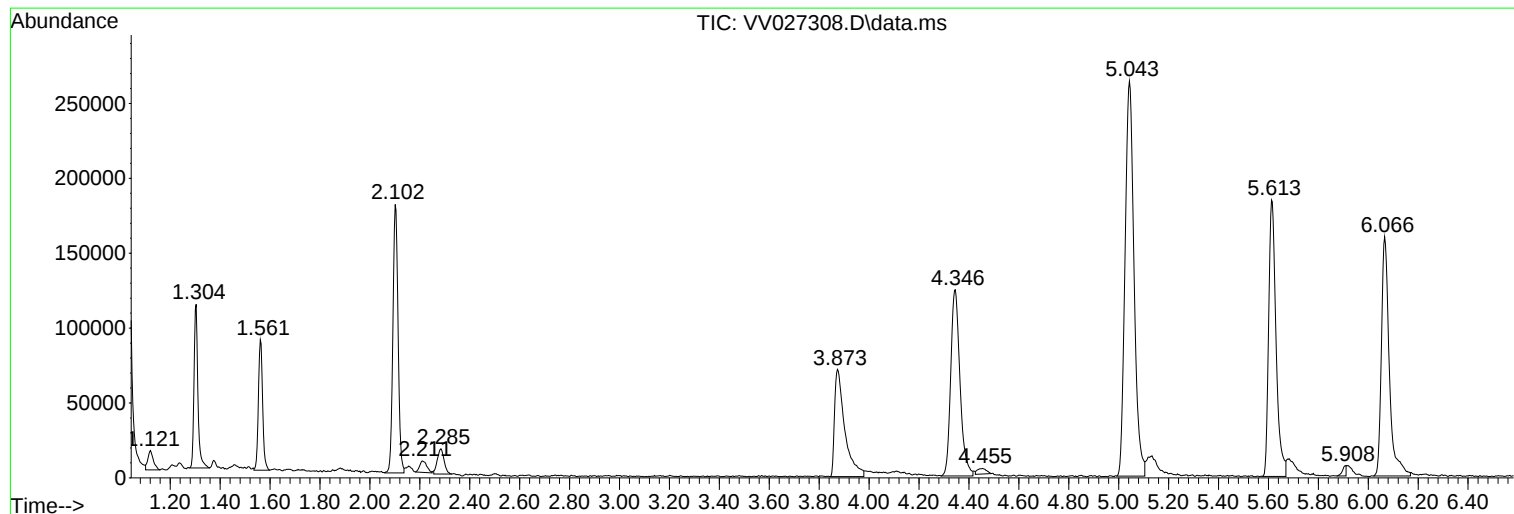

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027308.D
Acq On : 12 Aug 2022 04:21
Operator : SY/MD
Sample : N4162-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027308.D
Acq On : 12 Aug 2022 04:21
Operator : SY/MD
Sample : N4162-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc