

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027310.D
 Acq On : 12 Aug 2022 05:11
 Operator : SY/MD
 Sample : N4162-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	40	rVB	9702	15708	2.30%	0.300%
2	1.304	75	82	100	rVB	114247	122469	17.96%	2.336%
3	1.564	155	163	174	rBV	83265	97377	14.28%	1.857%
4	2.105	319	331	342	rBV	181600	264264	38.76%	5.041%
5	2.214	356	365	382	rVB3	8969	21517	3.16%	0.410%
6	3.883	875	884	910	rBV	65851	199140	29.21%	3.799%
7	4.342	1011	1027	1048	rBV	129041	315071	46.21%	6.010%
8	4.452	1055	1061	1075	rVB6	4512	9787	1.44%	0.187%
9	5.043	1229	1245	1266	rBV2	268307	681802	100.00%	13.005%
10	5.616	1411	1423	1439	rBV	187929	386353	56.67%	7.370%
11	6.066	1550	1563	1582	rBV	161901	342728	50.27%	6.538%
12	6.985	1839	1849	1865	rBV	62191	119400	17.51%	2.278%
13	7.313	1939	1951	1973	rBV	293216	536775	78.73%	10.239%
14	7.622	2038	2047	2070	rBV	36149	72511	10.64%	1.383%
15	8.088	2182	2192	2231	rBV2	252708	549038	80.53%	10.473%
16	8.850	2418	2429	2451	rBV	302050	508755	74.62%	9.704%
17	10.214	2841	2853	2867	rBV	105753	170356	24.99%	3.250%
18	11.249	3162	3175	3196	rBV	257539	410631	60.23%	7.833%
19	11.622	3279	3291	3312	rBV	253810	410201	60.16%	7.825%
20	14.152	4074	4078	4084	rVB	14831	8590	1.26%	0.164%




Sum of corrected areas: 5242473

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027310.D
Acq On : 12 Aug 2022 05:11
Operator : SY/MD
Sample : N4162-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

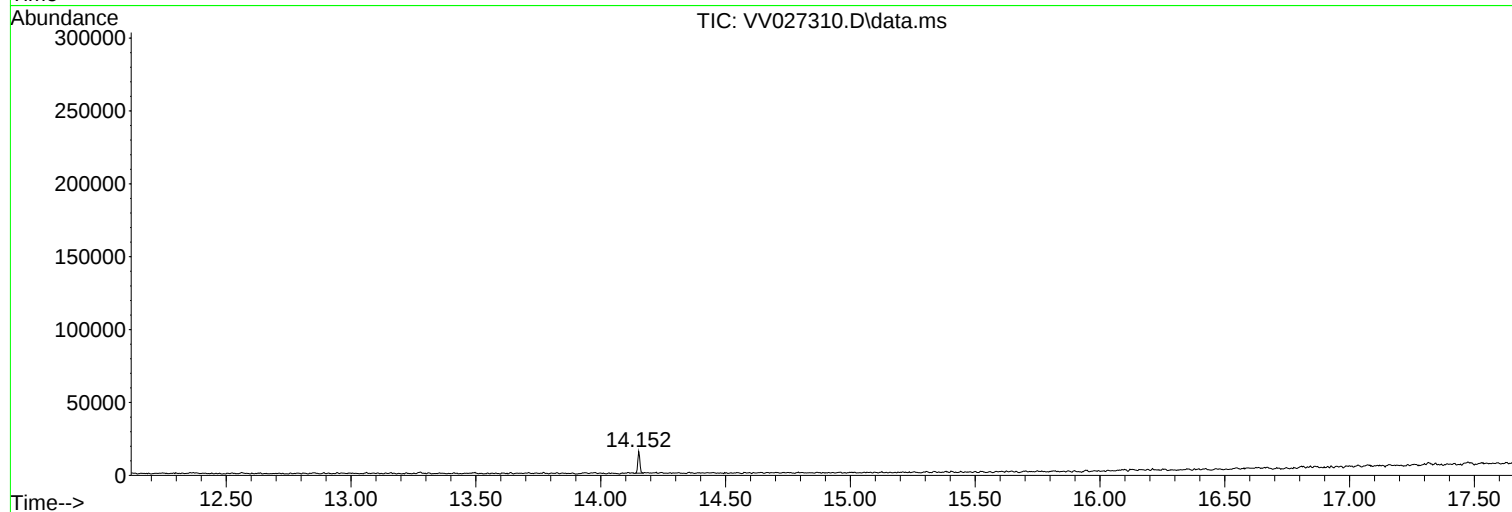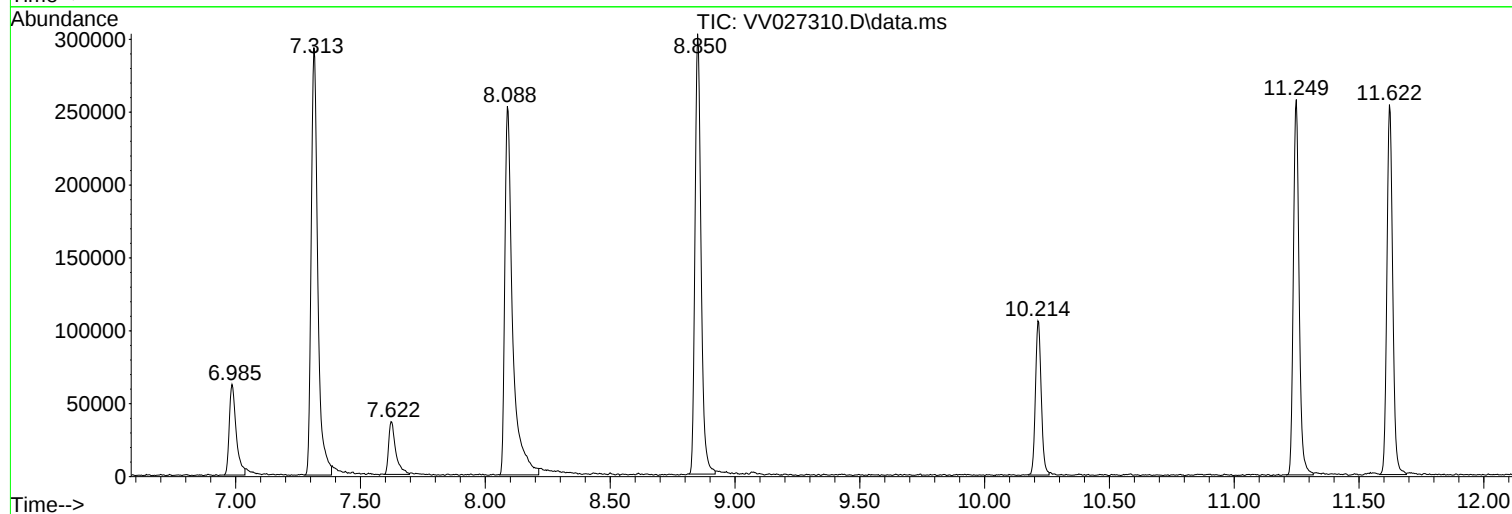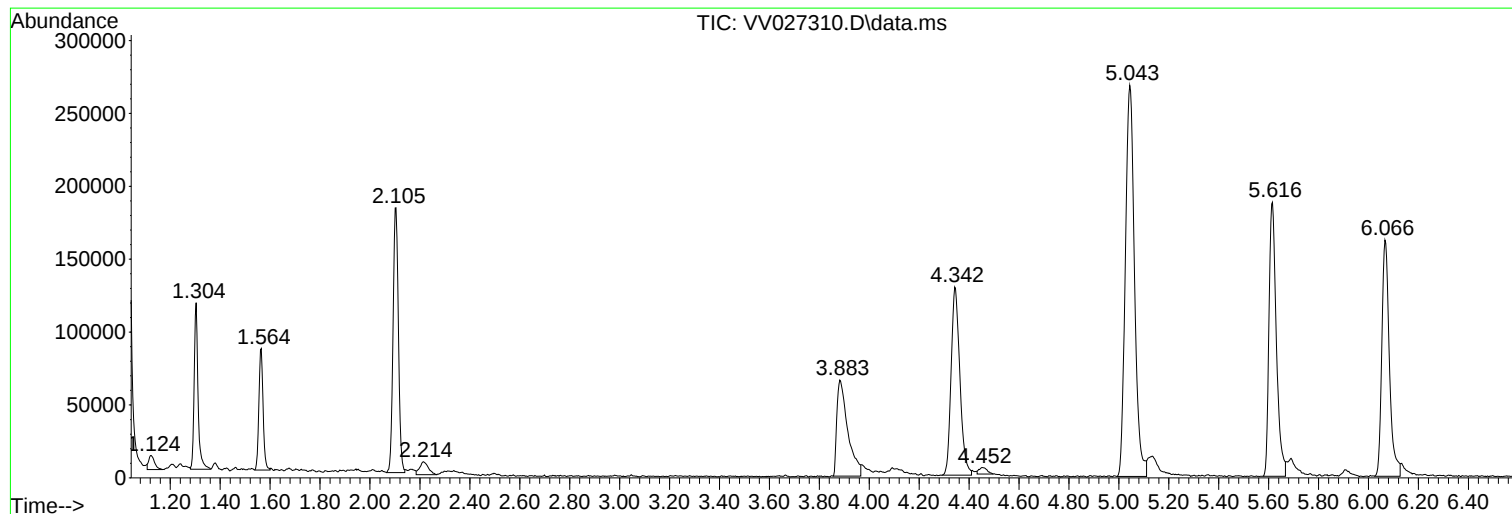

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027310.D
Acq On : 12 Aug 2022 05:11
Operator : SY/MD
Sample : N4162-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027310.D
Acq On : 12 Aug 2022 05:11
Operator : SY/MD
Sample : N4162-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
