

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027312.D
 Acq On : 12 Aug 2022 06:01
 Operator : SY/MD
 Sample : N4162-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	23	27	40	rVB	8816	12787	1.90%	0.223%
2	1.304	75	82	100	rVB	110024	118366	17.62%	2.064%
3	1.561	155	162	176	rVB	86368	101501	15.11%	1.770%
4	2.101	320	330	342	rBV	181366	258827	38.53%	4.513%
5	2.220	358	367	382	rVB3	8354	17798	2.65%	0.310%
6	3.879	873	883	915	rBV	70697	213159	31.73%	3.716%
7	4.092	942	949	955	rBV6	3851	6785	1.01%	0.118%
8	4.342	1012	1027	1051	rBV	123254	306915	45.69%	5.351%
9	5.043	1229	1245	1266	rBV2	270055	671794	100.00%	11.713%
10	5.137	1266	1274	1288	rVB4	10396	26988	4.02%	0.471%
11	5.612	1411	1422	1439	rBV	187084	386888	57.59%	6.745%
12	5.918	1505	1517	1533	rVB	4934	12313	1.83%	0.215%
13	6.066	1550	1563	1579	rBV	161327	335615	49.96%	5.851%
14	6.985	1837	1849	1876	rBV	58858	124548	18.54%	2.171%
15	7.313	1940	1951	1975	rBV	289137	533716	79.45%	9.305%
16	7.622	2037	2047	2069	rBV	36124	71946	10.71%	1.254%
17	7.937	2132	2145	2159	rBV	83128	155355	23.13%	2.709%
18	8.088	2181	2192	2225	rBV	252456	539783	80.35%	9.411%
19	8.850	2417	2429	2451	rBV	301725	516584	76.90%	9.007%
20	10.214	2842	2853	2869	rBV	103379	168444	25.07%	2.937%
21	10.381	2892	2905	2922	rVB	139941	243934	36.31%	4.253%
22	11.249	3165	3175	3201	rBV	263337	424117	63.13%	7.394%
23	11.622	3280	3291	3309	rBV	262597	414010	61.63%	7.218%
24	12.252	3476	3487	3499	rVB	43532	73463	10.94%	1.281%




Sum of corrected areas: 5735636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027312.D
Acq On : 12 Aug 2022 06:01
Operator : SY/MD
Sample : N4162-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

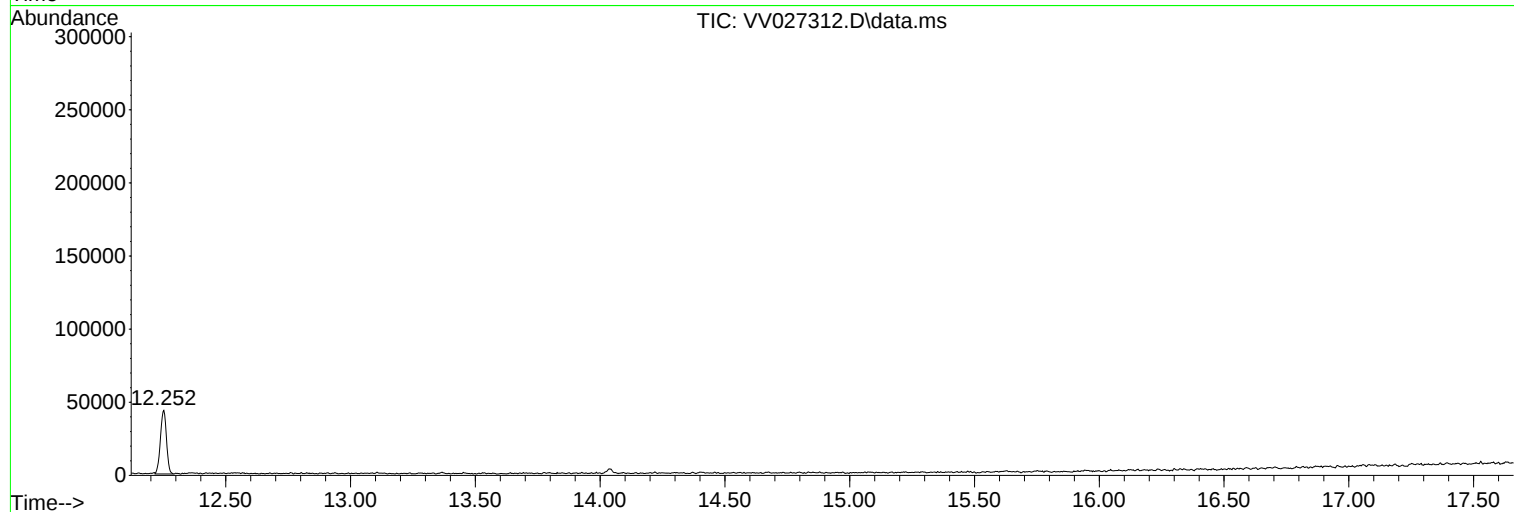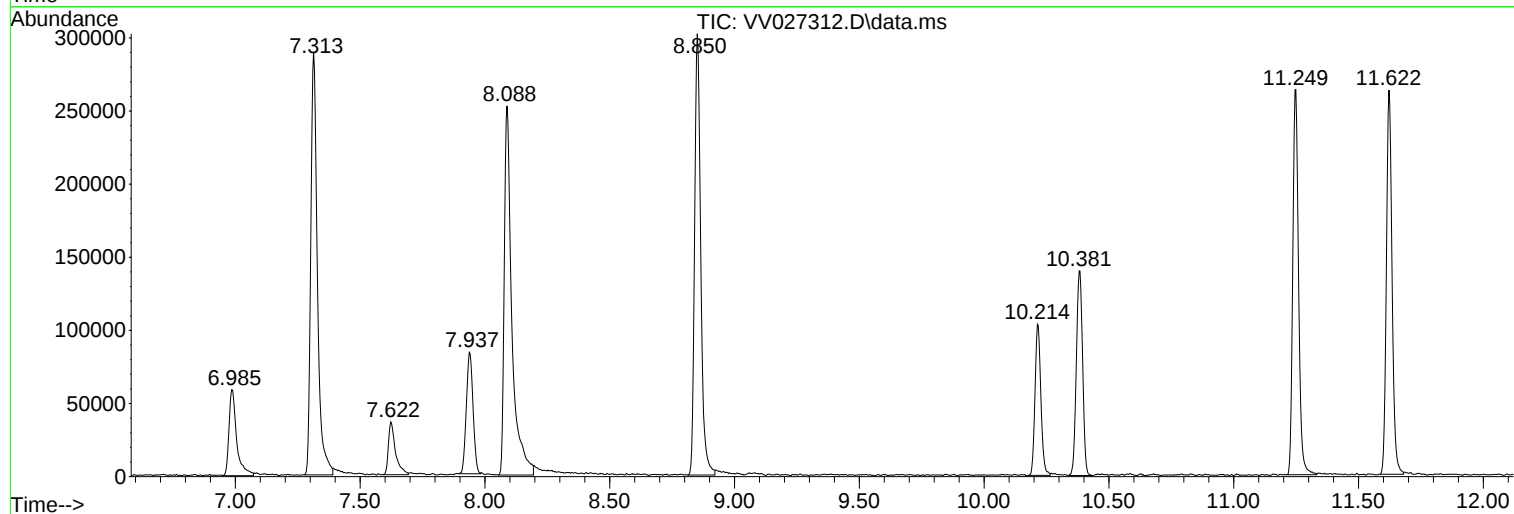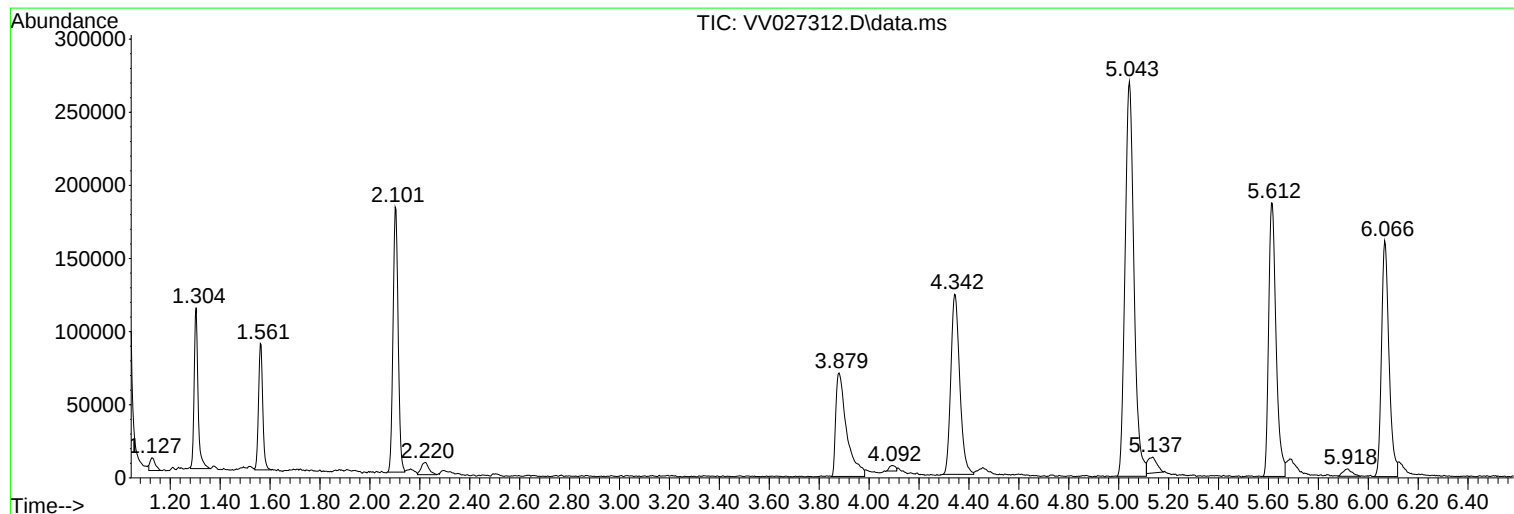

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027312.D
Acq On : 12 Aug 2022 06:01
Operator : SY/MD
Sample : N4162-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027312.D
Acq On : 12 Aug 2022 06:01
Operator : SY/MD
Sample : N4162-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
