

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027316.D
 Acq On : 12 Aug 2022 08:30
 Operator : SY/MD
 Sample : N4162-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBX5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	41	rVB	11287	14364	2.07%	0.271%
2	1.304	74	82	102	rBV	98310	116234	16.76%	2.193%
3	1.558	154	161	175	rVB	80083	94733	13.66%	1.788%
4	2.098	319	329	344	rBV	180536	260842	37.62%	4.922%
5	2.224	359	368	381	rBV3	7942	14645	2.11%	0.276%
6	3.883	874	884	918	rBV	73199	215687	31.11%	4.070%
7	4.343	1007	1027	1050	rBV	126391	324999	46.87%	6.132%
8	5.043	1229	1245	1266	rBV2	276644	693402	100.00%	13.084%
9	5.613	1410	1422	1441	rBV	193700	397982	57.40%	7.510%
10	6.066	1551	1563	1581	rBV	162877	344205	49.64%	6.495%
11	6.986	1835	1849	1868	rBV	62745	124731	17.99%	2.354%
12	7.313	1939	1951	1979	rBV	297809	547398	78.94%	10.329%
13	7.622	2038	2047	2067	rBV	37359	71934	10.37%	1.357%
14	7.940	2136	2146	2152	rBV4	4586	7041	1.02%	0.133%
15	8.088	2181	2192	2226	rBV	257083	543486	78.38%	10.255%
16	8.850	2417	2429	2448	rBV	302048	510470	73.62%	9.632%
17	10.214	2842	2853	2867	rBV	106586	173322	25.00%	3.270%
18	10.381	2897	2905	2914	rVB4	6565	9675	1.40%	0.183%
19	11.249	3164	3175	3201	rBV	265318	421325	60.76%	7.950%
20	11.622	3280	3291	3308	rBV	261419	413183	59.59%	7.796%




Sum of corrected areas: 5299658

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027316.D
Acq On : 12 Aug 2022 08:30
Operator : SY/MD
Sample : N4162-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

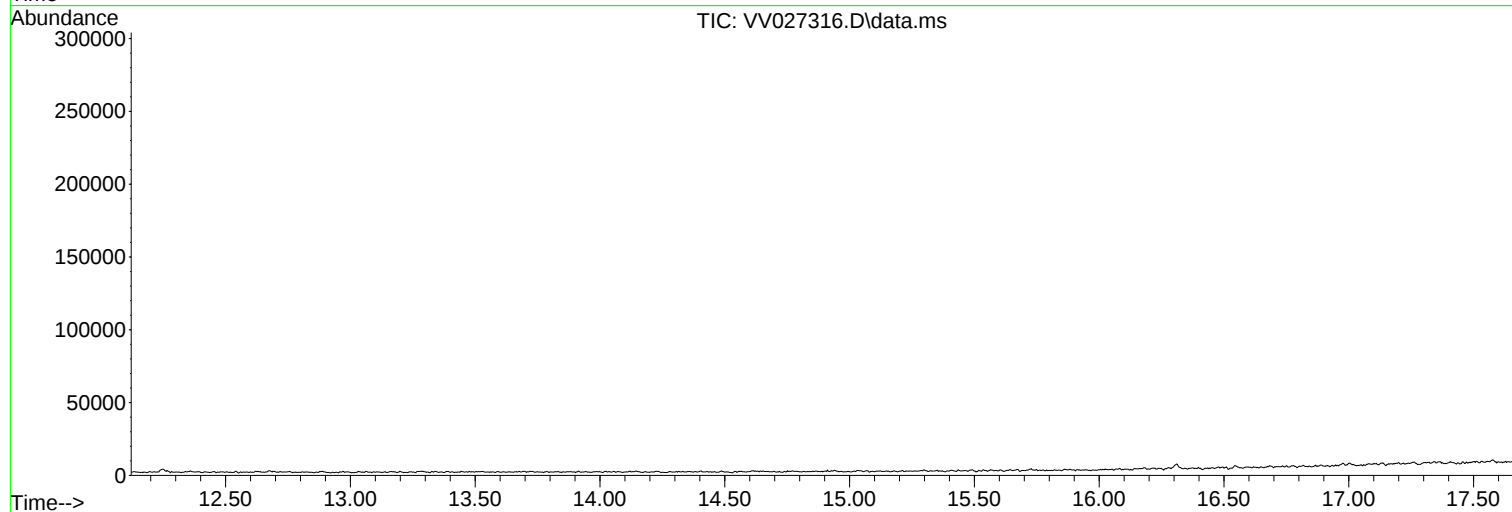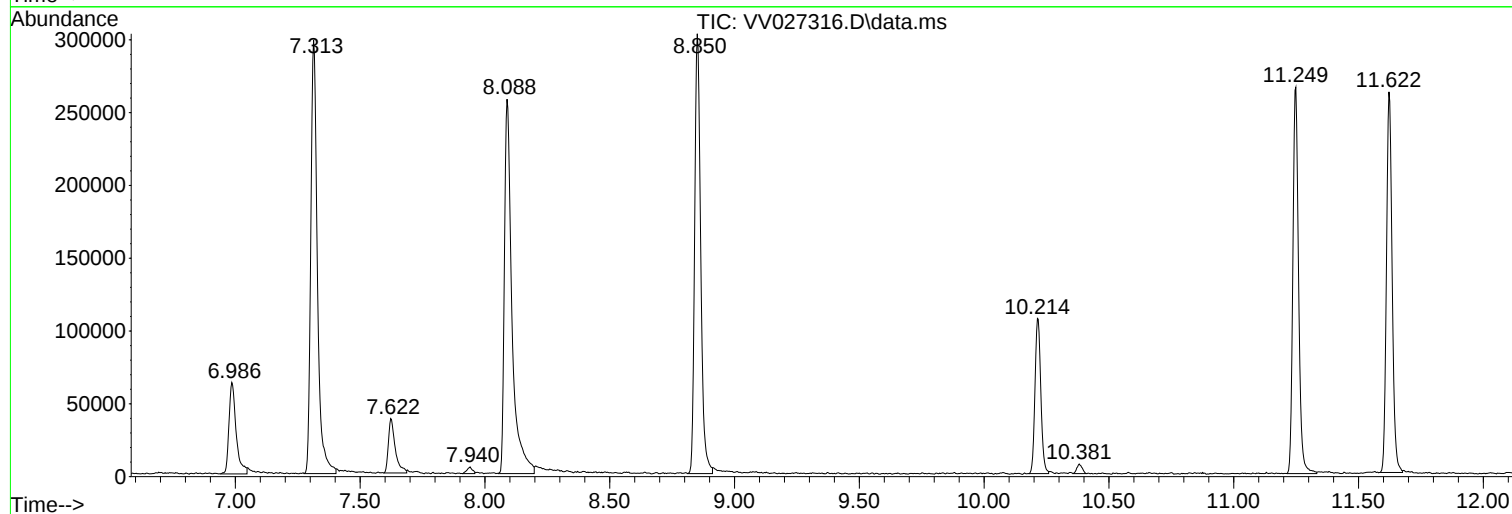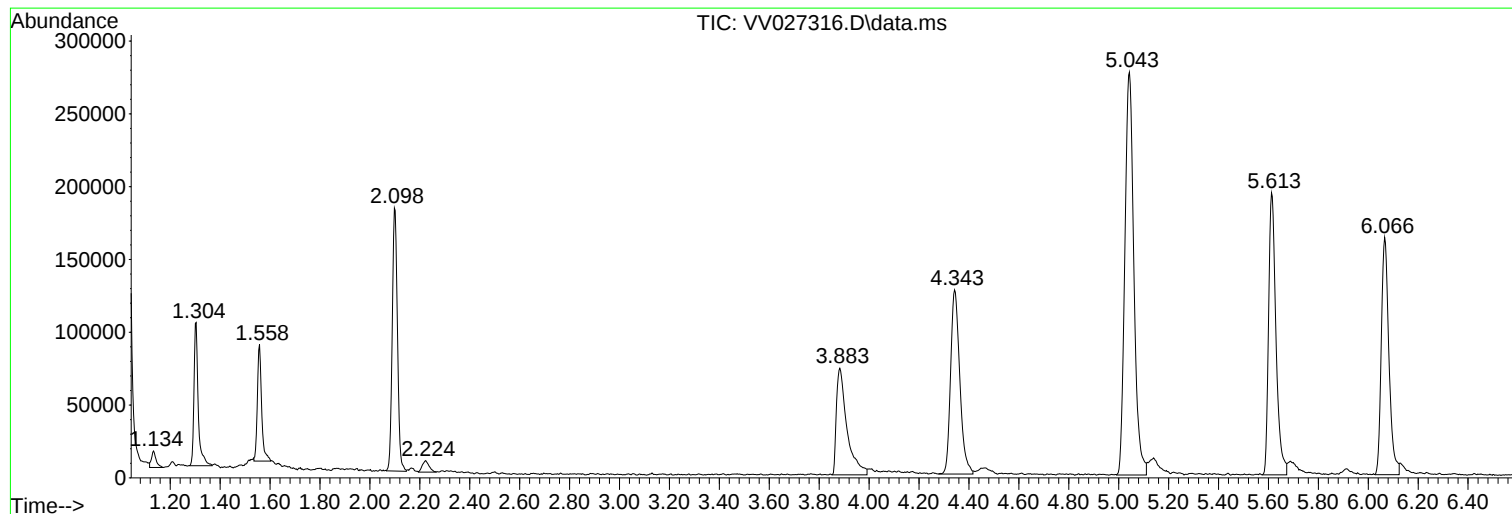

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027316.D
Acq On : 12 Aug 2022 08:30
Operator : SY/MD
Sample : N4162-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027316.D
Acq On : 12 Aug 2022 08:30
Operator : SY/MD
Sample : N4162-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc