

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
 Data File : VV027318.D
 Acq On : 12 Aug 2022 09:20
 Operator : SY/MD
 Sample : N4162-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGBZ9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	22	27	36	rVB	9473	11374	1.65%	0.215%
2	1.301	75	81	99	rBV	98806	113208	16.41%	2.139%
3	1.561	154	162	177	rBV	73916	90837	13.17%	1.716%
4	2.098	318	329	344	rBV	183873	263466	38.19%	4.978%
5	2.217	359	366	376	rVB4	8327	14692	2.13%	0.278%
6	3.886	876	885	922	rBV2	62700	209149	30.32%	3.952%
7	4.343	1010	1027	1052	rBV	127138	322608	46.76%	6.095%
8	5.040	1229	1244	1265	rBV2	276101	689876	100.00%	13.035%
9	5.613	1411	1422	1441	rBV	194787	403596	58.50%	7.626%
10	5.912	1501	1515	1526	rBV10	4149	9020	1.31%	0.170%
11	6.066	1550	1563	1578	rBV	161662	337242	48.88%	6.372%
12	6.986	1839	1849	1870	rBV	61487	122570	17.77%	2.316%
13	7.313	1940	1951	1975	rBV	289014	535053	77.56%	10.109%
14	7.622	2034	2047	2066	rBV2	35434	71051	10.30%	1.342%
15	7.937	2137	2145	2154	rBV5	4592	8064	1.17%	0.152%
16	8.088	2182	2192	2229	rBV	255240	543456	78.78%	10.268%
17	8.850	2417	2429	2457	rBV	307962	524814	76.07%	9.916%
18	10.214	2843	2853	2872	rBV	103836	171976	24.93%	3.249%
19	10.384	2895	2906	2918	rVB3	10455	16569	2.40%	0.313%
20	11.249	3163	3175	3199	rBV	263715	424467	61.53%	8.020%
21	11.622	3279	3291	3311	rBV	256080	409496	59.36%	7.737%




Sum of corrected areas: 5292584

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027318.D
Acq On : 12 Aug 2022 09:20
Operator : SY/MD
Sample : N4162-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

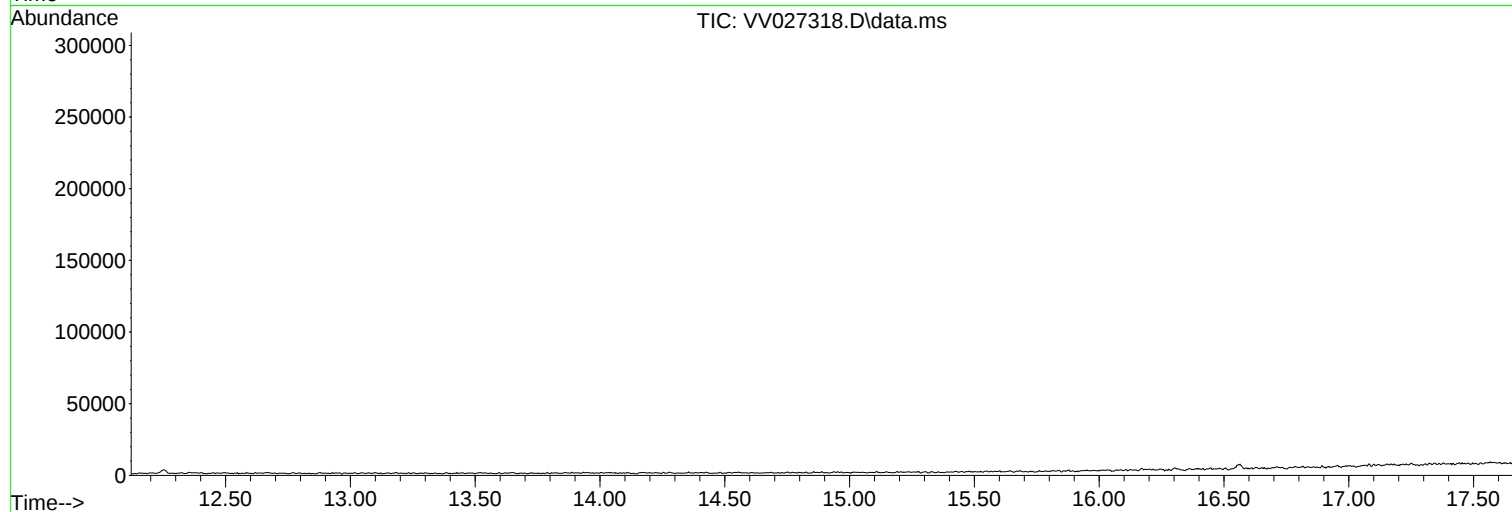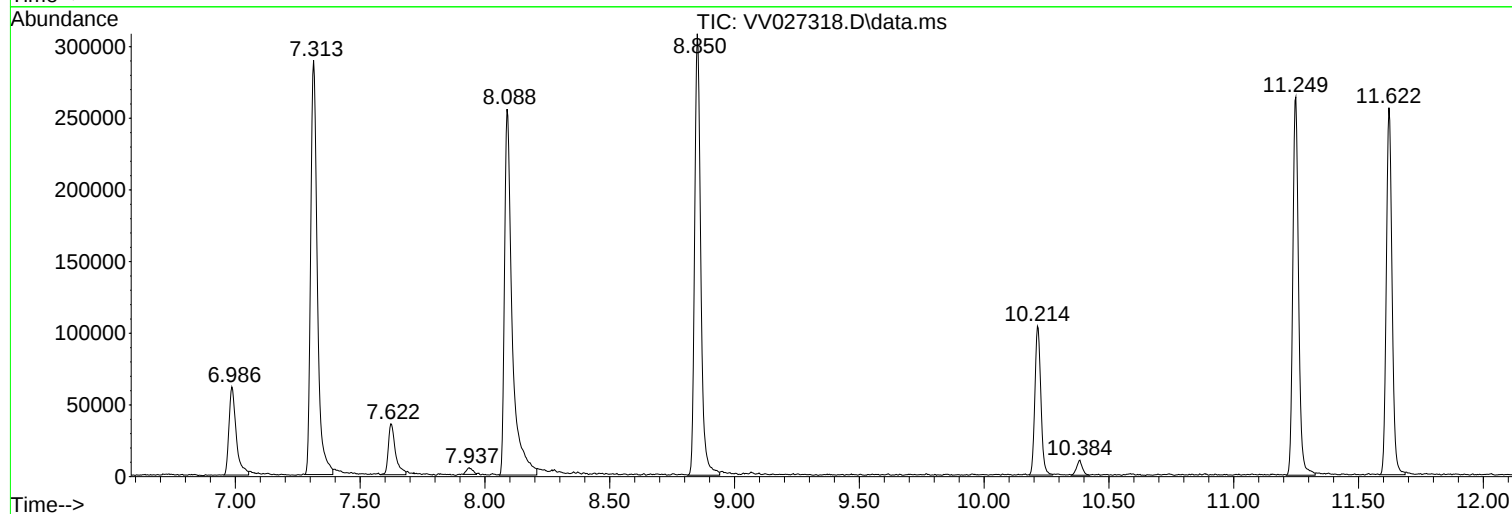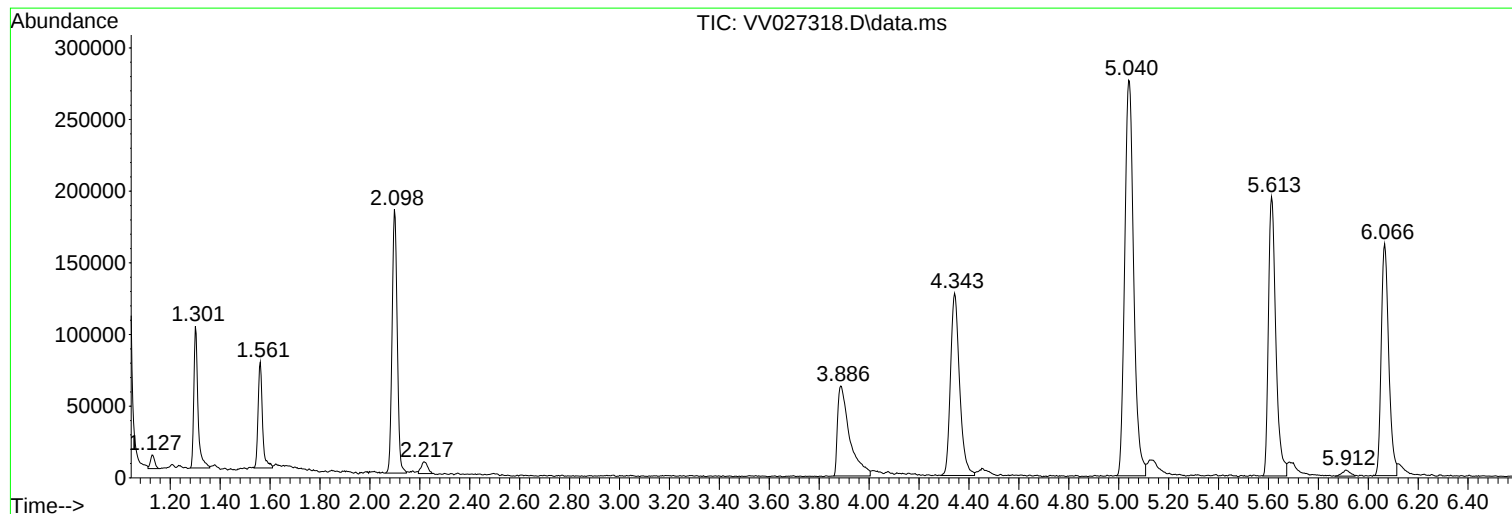

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027318.D
Acq On : 12 Aug 2022 09:20
Operator : SY/MD
Sample : N4162-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081222\
Data File : VV027318.D
Acq On : 12 Aug 2022 09:20
Operator : SY/MD
Sample : N4162-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGBZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc